

Sample Name : β -Amyloid (25-35)
 Cat No. : RP10008
 Lot No. : PE3881604

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
31.00	Pumps	Pump B Conc.	95
31.01	Pumps	Pump B Conc.	5
39.00	Pumps	Pump B Conc.	5
39.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

<Chromatogram>

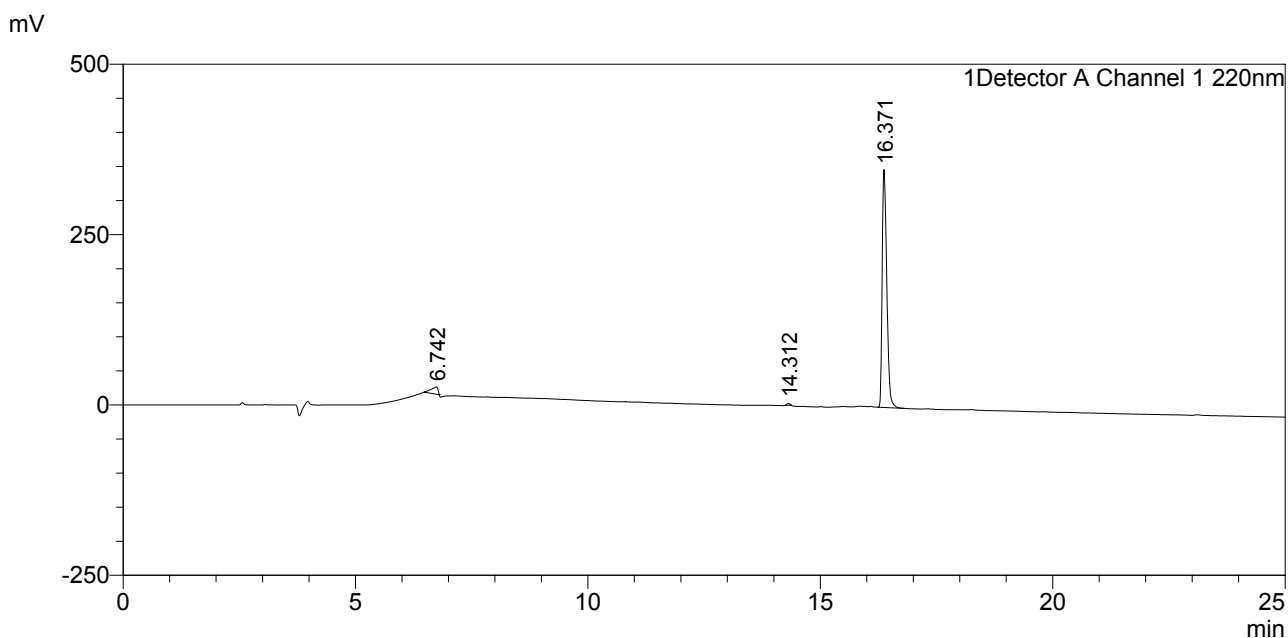

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	6.742	106811	10681	4.242
2	14.312	11885	2670	0.472
3	16.371	2398989	348774	95.286
Total		2517684	362125	100.000