

Sample Name : HA Peptide
 Cat. No. : RP11735
 Lot. No. : PE8041606

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

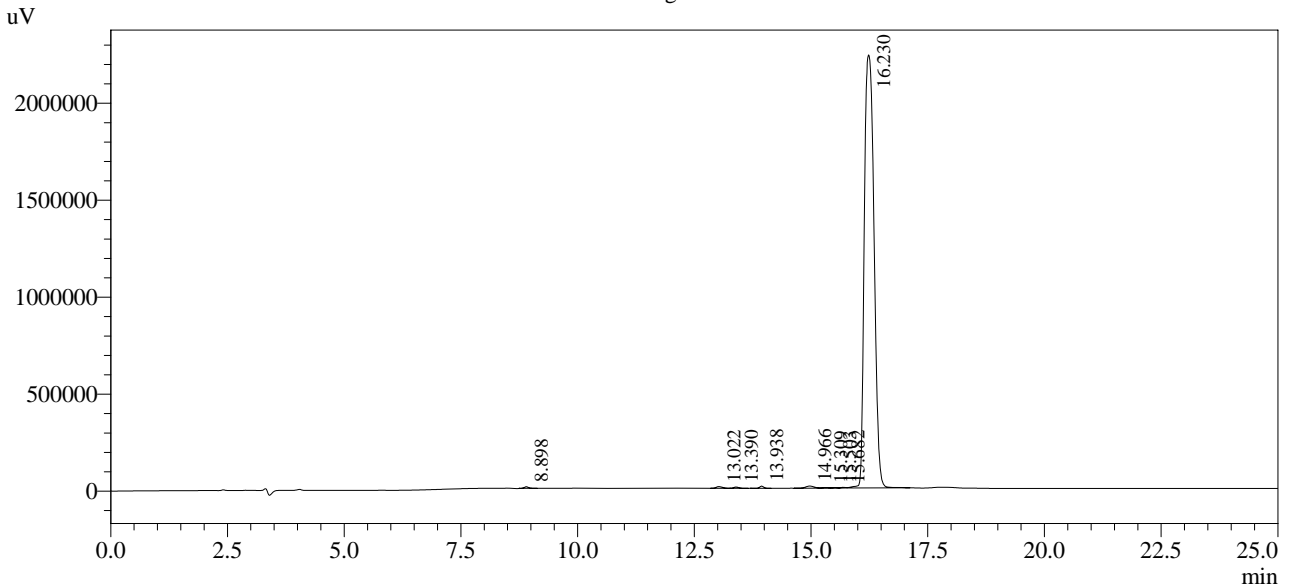

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.898	44817	7747	0.137
2	13.022	82112	8564	0.252
3	13.390	50448	6436	0.155
4	13.938	70246	11405	0.215
5	14.966	136482	10597	0.418
6	15.309	24096	2413	0.074
7	15.503	17932	2166	0.055
8	15.682	25042	3758	0.077
9	16.230	32183419	2233133	98.617
Total		32634593	2286219	100.000