

Sample Name :hgp100(25-33)  
 Cat. No. :RP20344  
 Lot. No. : PE4691606

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

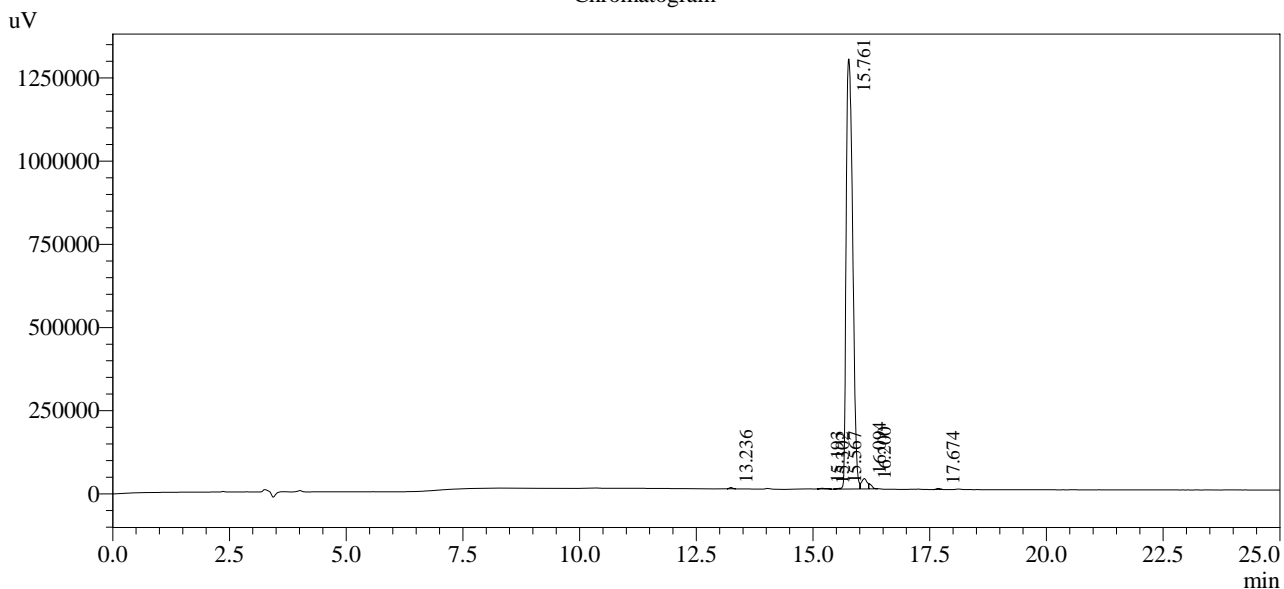

I Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.236	19449	3983	0.150
2	15.193	12733	2227	0.099
3	15.302	6495	1284	0.050
4	15.567	10349	2441	0.080
5	15.761	12534325	1292533	96.990
6	16.094	259208	31297	2.006
7	16.200	66562	15390	0.515
8	17.674	14182	2858	0.110
Total		12923303	1352015	100.000