

Sample Name :HA Peptide
 Cat. No. : RP11735
 Lot. No. : PE7201701

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

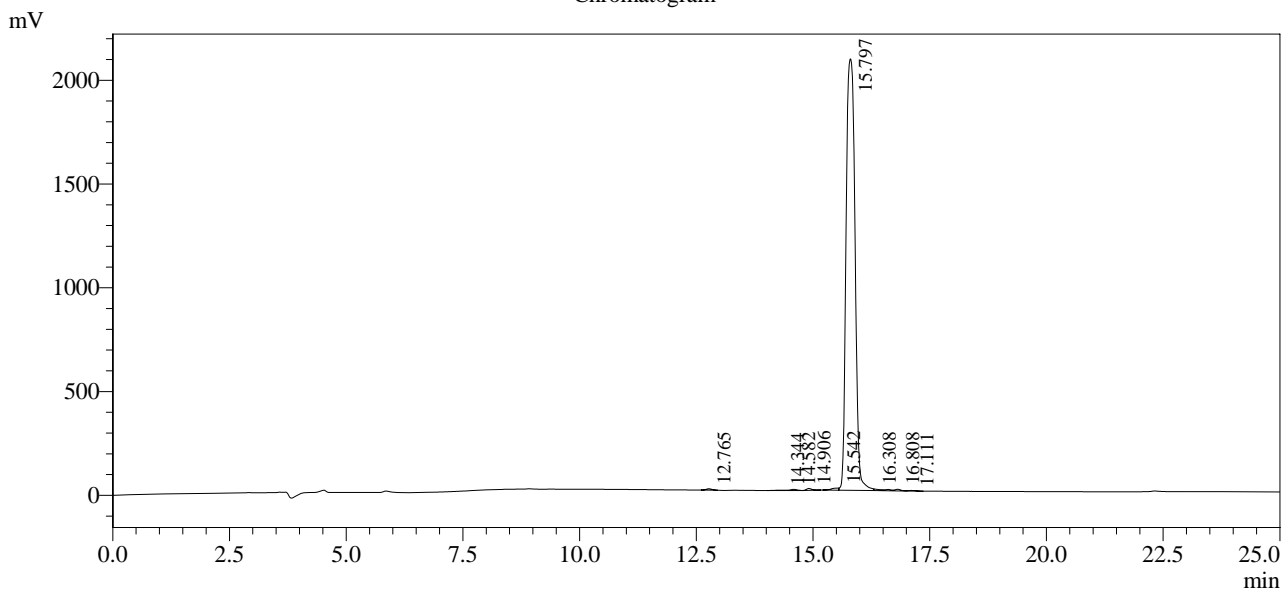

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.765	56049	6367	0.199
2	14.344	21977	1404	0.078
3	14.582	53786	5288	0.191
4	14.906	74206	8848	0.263
5	15.542	110223	10373	0.391
6	15.797	27632178	2079287	98.054
7	16.308	127182	8106	0.451
8	16.808	71777	7543	0.255
9	17.111	33219	2795	0.118
Total		28180596	2130012	100.000