

Sample Name :HA Peptide
 Cat No :RP11735
 Lot No :E2264321A
 Time Processed :12:03:04 PM
 Month-Day-Year Processed :01/24/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: SS-CM-0309

<Chromatogram>

mV

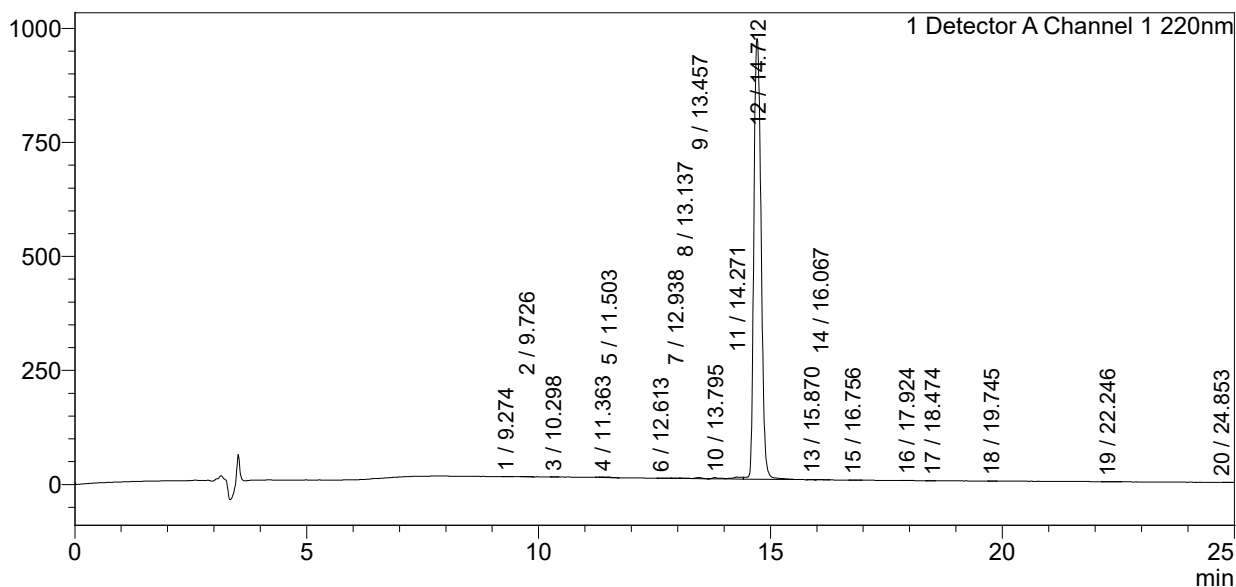

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.274	1359	218	0.013
2	9.726	1871	263	0.018
3	10.298	1005	133	0.009
4	11.363	11898	1558	0.112
5	11.503	10311	1425	0.097
6	12.613	1315	161	0.012
7	12.938	2166	314	0.020
8	13.137	3209	367	0.030
9	13.457	20824	2405	0.197
10	13.795	28410	2936	0.269
11	14.271	64754	4235	0.612
12	14.712	10413088	965939	98.438
13	15.870	2732	520	0.026
14	16.067	5790	695	0.055
15	16.756	1342	101	0.013
16	17.924	1296	174	0.012

Peak#	Ret. Time	Area	Height	Area%
17	18.474	1276	225	0.012
18	19.745	1043	189	0.010
19	22.246	3063	350	0.029
20	24.853	1527	202	0.014
Total		10578280	982409	100.000