

Sample Name :HA Peptide
 Cat. No. : RP11735
 Lot. No. : PE3121704

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

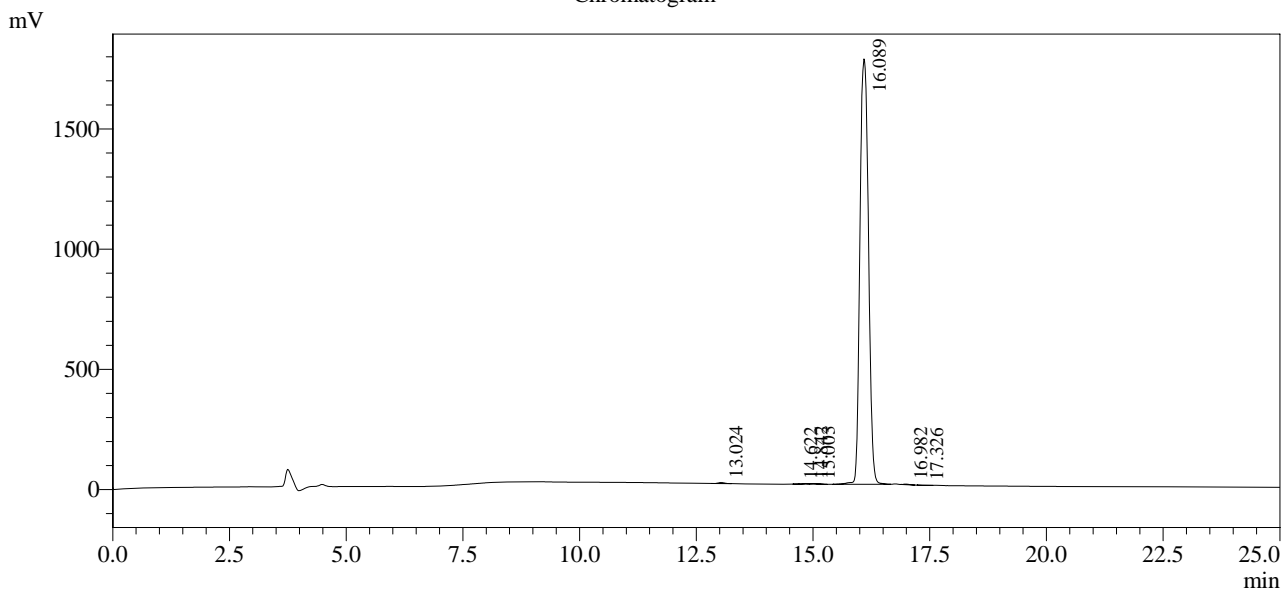

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.024	41894	4409	0.184
2	14.622	485	116	0.002
3	14.842	22691	2588	0.100
4	15.003	36244	3092	0.160
5	16.089	22585496	1769669	99.423
6	16.982	20518	2718	0.090
7	17.326	9286	855	0.041
Total		22716615	1783446	100.000