

Sample Information

Sample Name :Neuropeptide Y, human  
 Sample ID :U0626CL270-1

Pump A : 0.065% trifluoroacetic in 100% waters (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)


<<Pump>>  
 Flow : 1.0000 mL/min

<<Detector A>>  
 Wavelength Ch1 : 220 nm

<<LC Time Program>>

Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	5	
25.00	Pumps	Solvent B Conc.	65	
25.01	Pumps	Solvent B Conc.	95	
27.00	Pumps	Solvent B Conc.	95	
27.01	Pumps	Solvent B Conc.	5	
35.00	Pumps	Solvent B Conc.	5	
35.01	Controller	Stop		

<<Column Performance>>  
 <Detector A>  
 Column : Inertsil ODS-3 4.6 x 250 mm

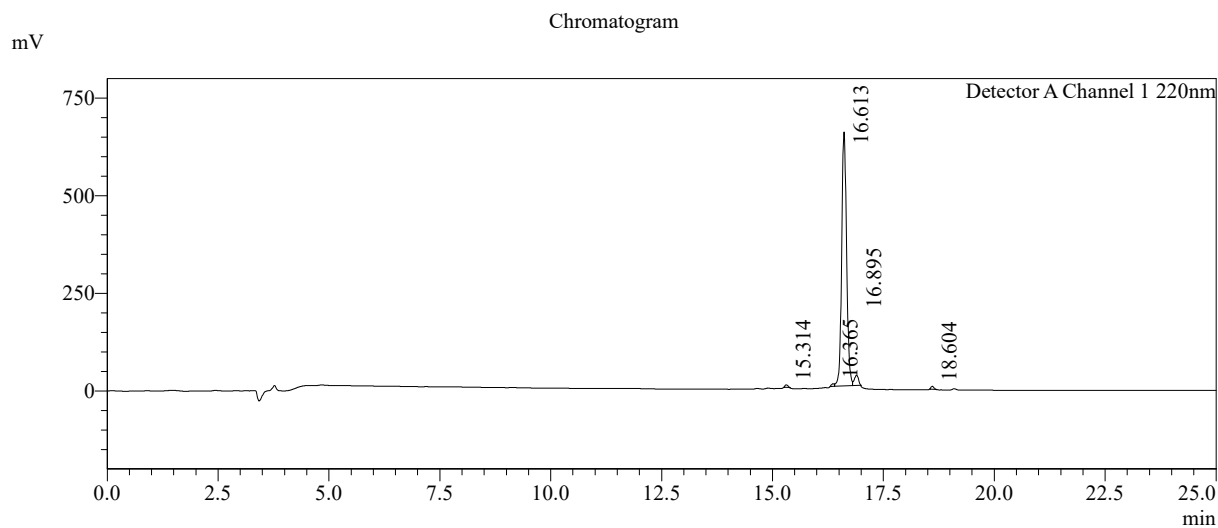

Peak Table

Peak#	Ret. Time	Height	Area	Height%	Area%
1	15.314	6212	27627	0.891	0.522
2	16.365	6578	31095	0.943	0.587
3	16.613	650322	5031460	93.266	95.044
4	16.895	26244	166808	3.764	3.151
5	18.604	7923	36842	1.136	0.696
Total		697279	5293831	100.000	100.000