

Sample Name :HA Peptide
 Cat. No. : RP11735
 Lot. No. : E4666619I
 Time Processed :9:05:14
 Month-Day-Year Processed :09/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

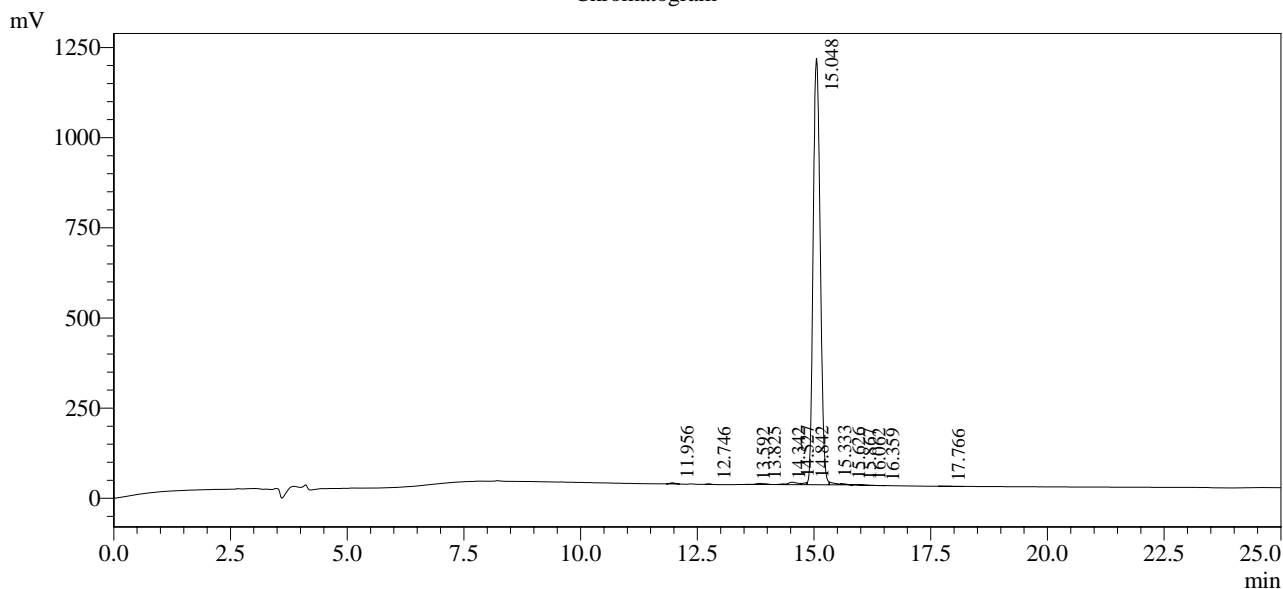

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.956	22508	2940	0.176
2	12.746	7802	1532	0.061
3	13.592	3689	486	0.029
4	13.825	45507	3277	0.356
5	14.342	15935	1871	0.125
6	14.527	90321	6789	0.706
7	14.842	34843	5533	0.272
8	15.048	12475381	1182565	97.504
9	15.333	71765	7249	0.561
10	15.626	7106	936	0.056
11	15.867	2788	604	0.022
12	16.062	7024	1043	0.055
13	16.359	5540	719	0.043
14	17.766	4476	448	0.035
Total		12794685	1215992	100.000