

Sample Name:HA Peptide
 Cat No :RP11735
 Lot No :E1944421E
 Time Processed :3:33:43 PM
 Month-Day-Year Processed :05/13/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: SS-CM-0309

<Chromatogram>

mV

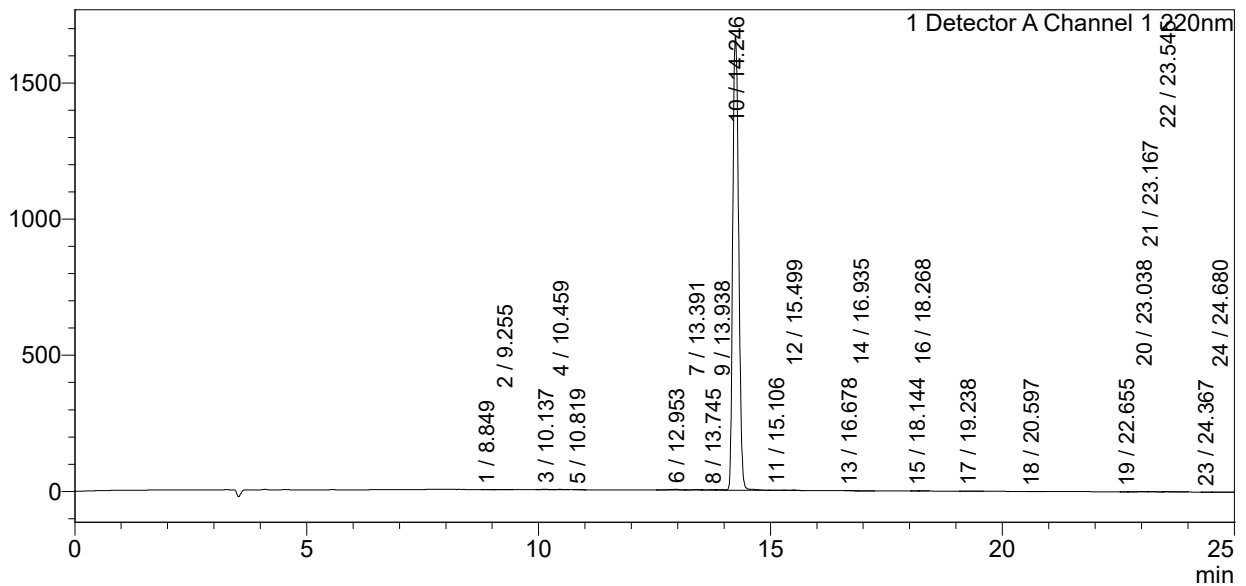

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.849	1124	145	0.007
2	9.255	4549	400	0.030
3	10.137	15877	1967	0.105
4	10.459	9497	1381	0.063
5	10.819	1001	127	0.007
6	12.953	34138	2690	0.226
7	13.391	15079	1483	0.100
8	13.745	22005	2002	0.146
9	13.938	20469	1916	0.136
10	14.246	14882112	1670510	98.598
11	15.106	6624	711	0.044
12	15.499	16824	1520	0.111
13	16.678	1880	231	0.012
14	16.935	1252	93	0.008
15	18.144	1138	187	0.008
16	18.268	2263	352	0.015

Peak#	Ret. Time	Area	Height	Area%
17	19.238	3831	364	0.025
18	20.597	2468	210	0.016
19	22.655	1208	169	0.008
20	23.038	17930	1120	0.119
21	23.167	14600	1052	0.097
22	23.545	13222	1109	0.088
23	24.367	1035	146	0.007
24	24.680	3552	195	0.024
Total		15093678	1690082	100.000