

Sample Name : Glucagon (1-29), Human  
 Cat. No. : RP10772  
 Lot. No. : PE4371903  
 Time Processed : 12:44:32  
 Month-Day-Year Processed : 03/13/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

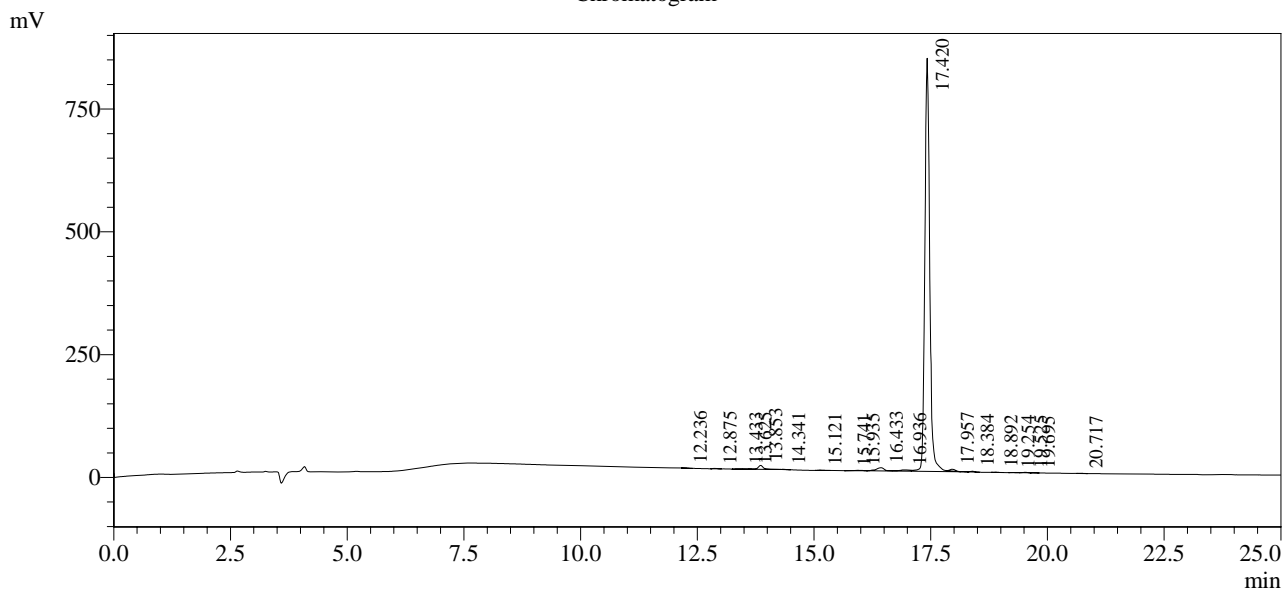

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.236	3348	606	0.052
2	12.875	5646	1071	0.088
3	13.433	2386	295	0.037
4	13.625	7632	731	0.118
5	13.853	61307	7850	0.950
6	14.341	2170	391	0.034
7	15.121	5196	643	0.081
8	15.741	1814	264	0.028
9	15.935	8840	836	0.137
10	16.433	81369	6534	1.261
11	16.936	44097	3040	0.684
12	17.420	6174491	841235	95.723
13	17.957	28381	3560	0.440
14	18.384	9941	1658	0.154
15	18.892	3115	428	0.048
16	19.254	1373	181	0.021
17	19.525	5502	860	0.085
18	19.695	1360	266	0.021
19	20.717	2411	379	0.037
Total		6450378	870827	100.000