

Sample Name : Calcitonin Gene Related Peptide (CGRP), rat
 Cat No. : RP11095
 Lot No. : PE7941902
 Time Processed : 7:36:21
 Month-Day-Year Processed : 03/01/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK12010012

<Chromatogram>

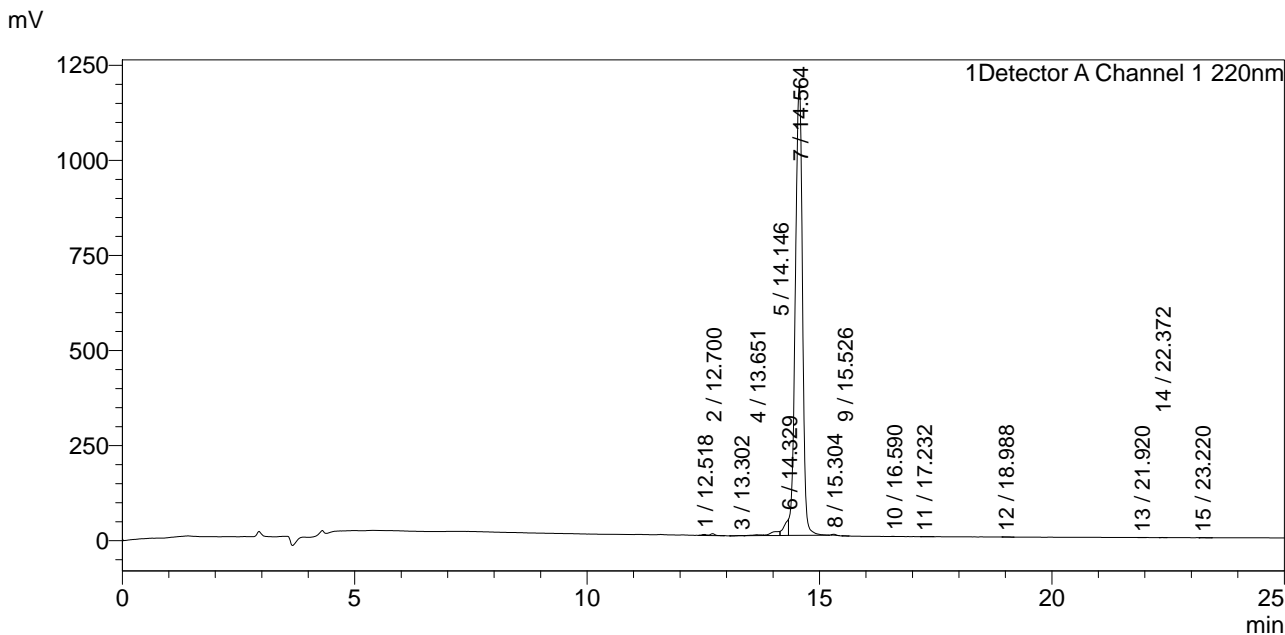

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.518	17266	2772	0.131
2	12.700	33826	4933	0.256
3	13.302	4717	465	0.036
4	13.651	35795	2260	0.271
5	14.146	142692	10716	1.081
6	14.329	286697	40751	2.172
7	14.564	12652714	1182845	95.875
8	15.304	11215	2217	0.085
9	15.526	1171	284	0.009
10	16.590	2128	288	0.016
11	17.232	2421	227	0.018
12	18.988	2093	226	0.016
13	21.920	1717	199	0.013
14	22.372	1466	299	0.011
15	23.220	1193	192	0.009

Peak#	Ret. Time	Area	Height	Area%
Total		13197111	1248674	100.000