

Sample Name : SV40 T-Ag-derived NLS peptide
 Cat. No. : RP20513
 Lot. No. : PE1791905
 Time Processed :13:25:21
 Month-Day-Year Processed :05/24/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

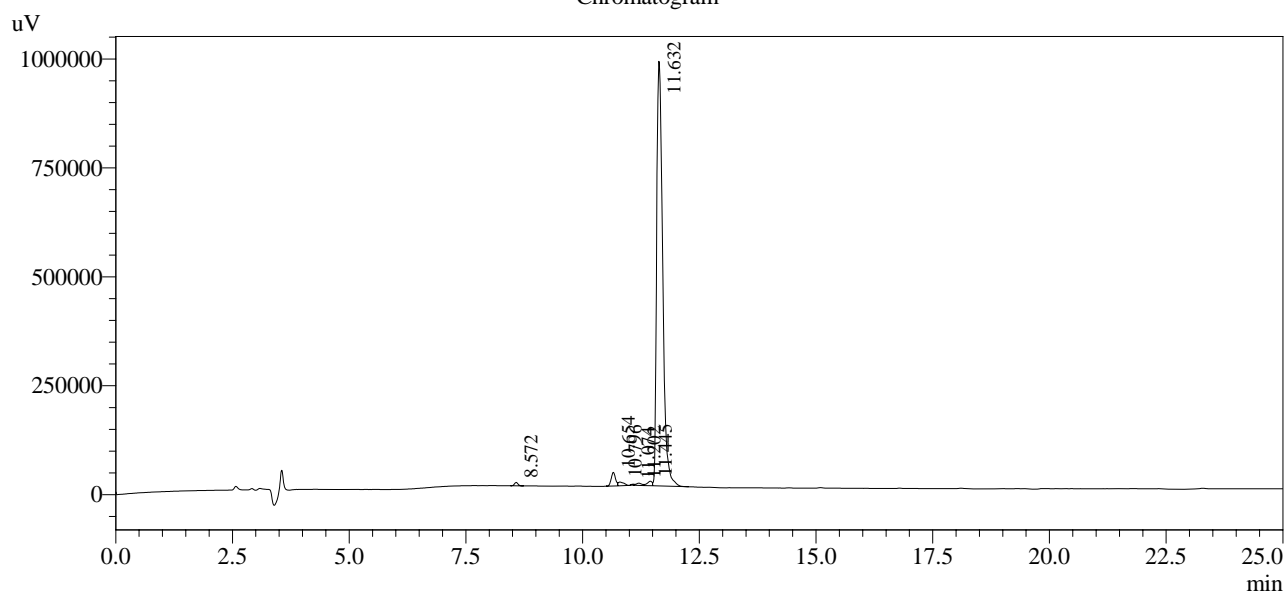

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.572	40696	7717	0.442
2	10.654	199757	31327	2.172
3	10.796	71589	8512	0.778
4	11.074	9721	2644	0.106
5	11.202	43552	5151	0.473
6	11.445	76199	10426	0.828
7	11.632	8757135	974727	95.200
Total		9198649	1040504	100.000