

Sample Name: β -Amyloid (25-35)
 Cat. No. : RP10008
 Lot. No. : E8128621B
 Time Processed :22:13:30
 Month-Day-Year Processed :02/20/2021
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ20010140

<Chromatogram>

mV

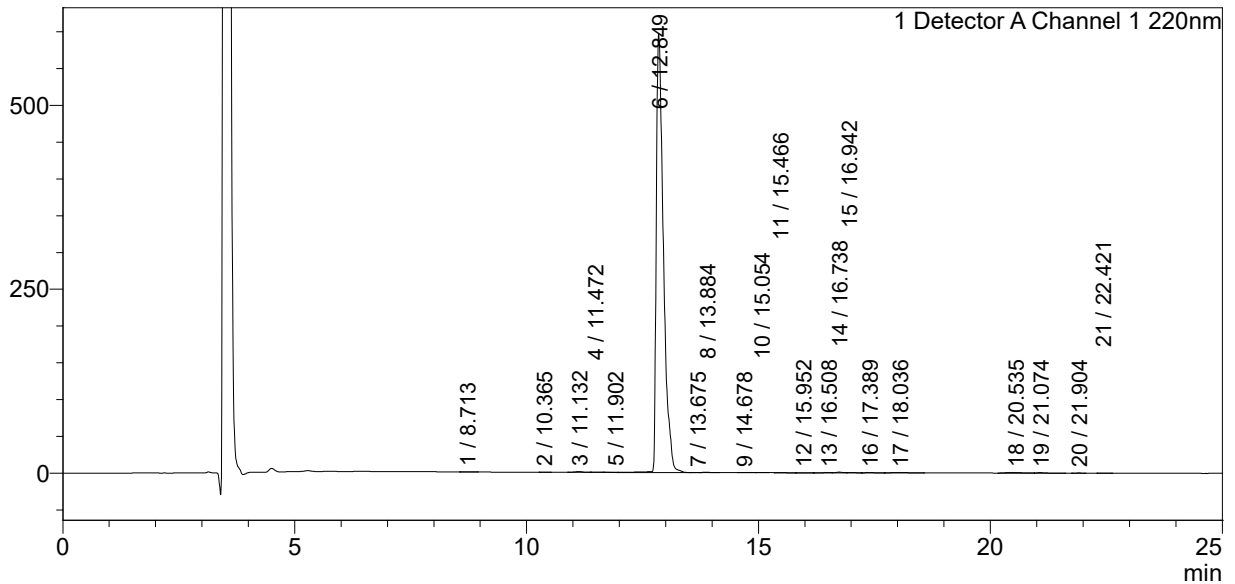

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.713	1187	82	0.018
2	10.365	1285	157	0.020
3	11.132	13682	1233	0.210
4	11.472	1694	201	0.026
5	11.902	3092	302	0.047
6	12.849	6409612	596891	98.441
7	13.675	1746	212	0.027
8	13.884	5218	489	0.080
9	14.678	1819	169	0.028
10	15.054	1262	185	0.019
11	15.466	2455	190	0.038
12	15.952	1404	108	0.022
13	16.508	3133	241	0.048
14	16.738	10152	1032	0.156
15	16.942	3338	234	0.051
16	17.389	4900	260	0.075

Peak#	Ret. Time	Area	Height	Area%
17	18.036	11175	508	0.172
18	20.535	21667	686	0.333
19	21.074	9168	804	0.141
20	21.904	2047	229	0.031
21	22.421	1061	115	0.016
Total		6511097	604326	100.000