

Sample Name :Neuropeptide Y, human
 Cat No.: RP10492
 Lot No.: E4975720B
 Time Processed :10:44:48
 Month-Day-Year Processed :02/12/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

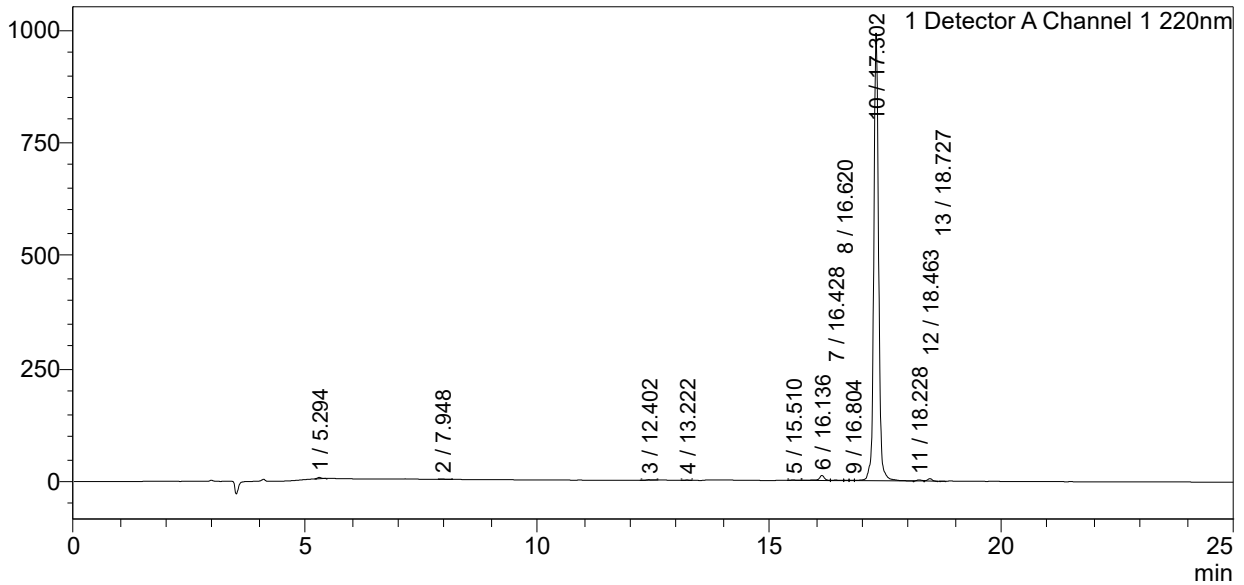

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.294	16511	2977	0.224
2	7.948	3400	740	0.046
3	12.402	6256	988	0.085
4	13.222	3199	544	0.043
5	15.510	6482	839	0.088
6	16.136	92200	11060	1.253
7	16.428	11590	1184	0.158
8	16.620	4702	635	0.064
9	16.804	5134	755	0.070
10	17.302	7153731	990810	97.228
11	18.228	17802	2423	0.242
12	18.463	36207	5574	0.492
13	18.727	500	107	0.007
Total		7357714	1018636	100.000