

Sample Name :Glucagon (1-29), Human  
 Cat. No. : RP10772  
 Lot. No. : PE7941902  
 Time Processed : 15:45:48  
 Month-Day-Year Processed : 03/03/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

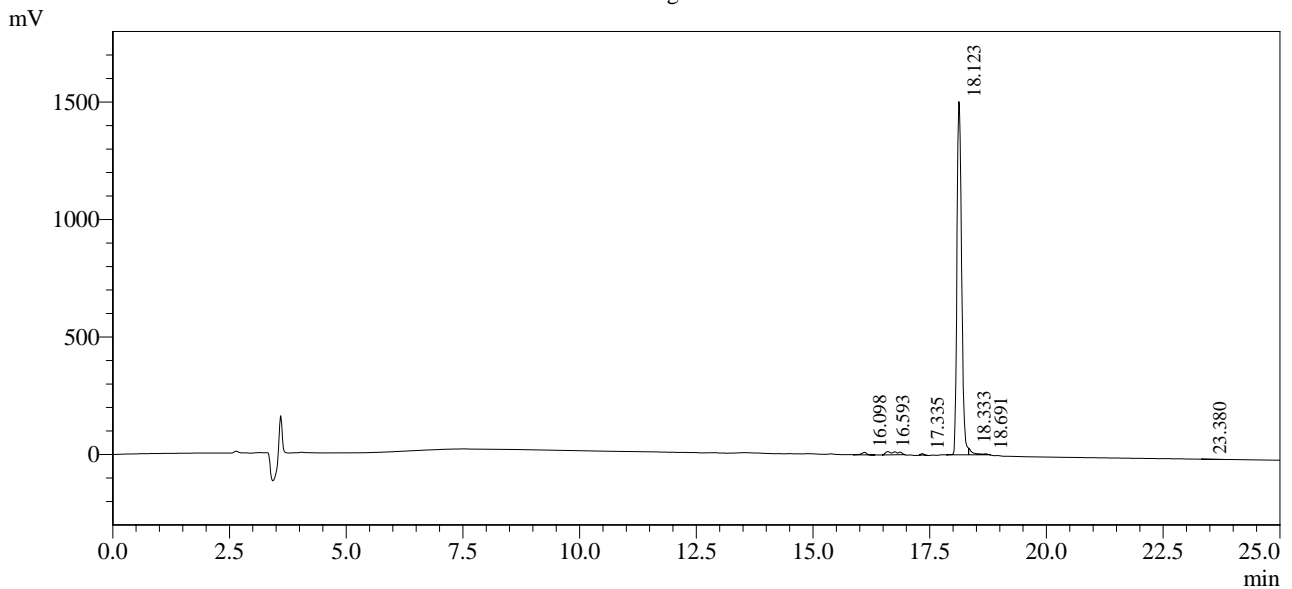

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	16.098	81037	11047	0.738
2	16.593	242125	14001	2.206
3	17.335	28698	6085	0.262
4	18.123	10446074	1503306	95.188
5	18.333	147081	28475	1.340
6	18.691	24072	3893	0.219
7	23.380	5106	251	0.047
Total		10974194	1567058	100.000