

Sample Name : Calcitonin Gene Related Peptide (CGRP), rat  
 Cat No : RP11095  
 Lot No : E2690521A  
 Time Processed : 1:17:30 PM  
 Month-Day-Year Processed : 01/06/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment : SS-CM-0309

<Chromatogram>

mV

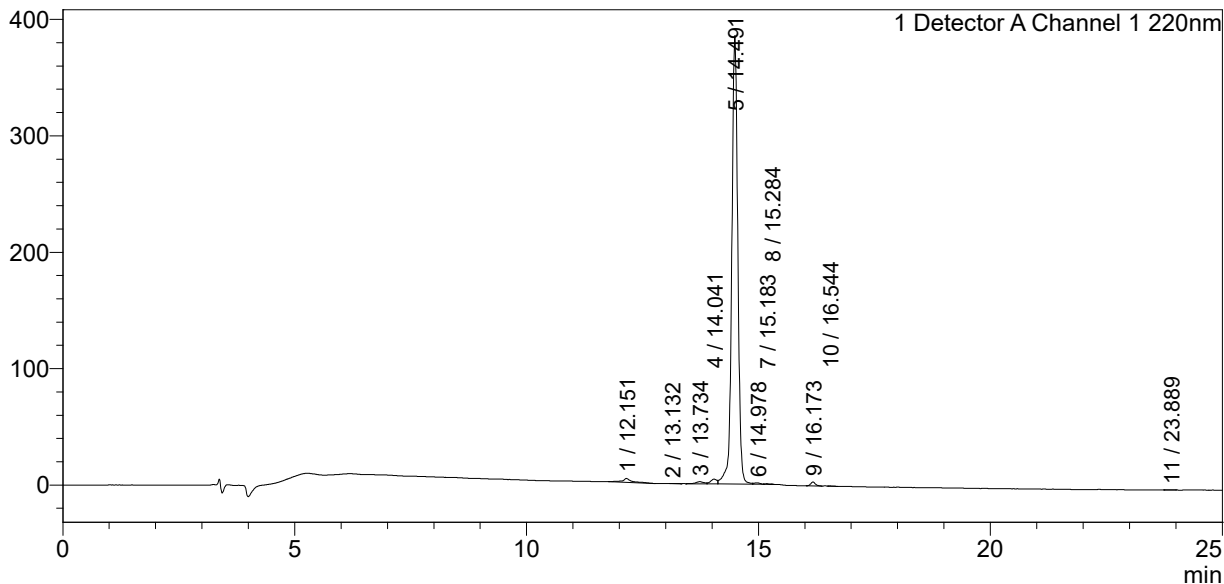

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.151	49487	3372	1.364
2	13.132	1982	192	0.055
3	13.734	24122	1858	0.665
4	14.041	39575	4173	1.091
5	14.491	3472819	385352	95.697
6	14.978	10476	1076	0.289
7	15.183	2979	588	0.082
8	15.284	1899	401	0.052
9	16.173	23407	3383	0.645
10	16.544	1384	234	0.038
11	23.889	835	119	0.023
Total		3628966	400747	100.000