

Sample Name : β -Amyloid (25-35)
 Cat. No. : RP10008
 Lot. No. : E2615720G
 Time Processed :16:18:50
 Month-Day-Year Processed :07/30/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

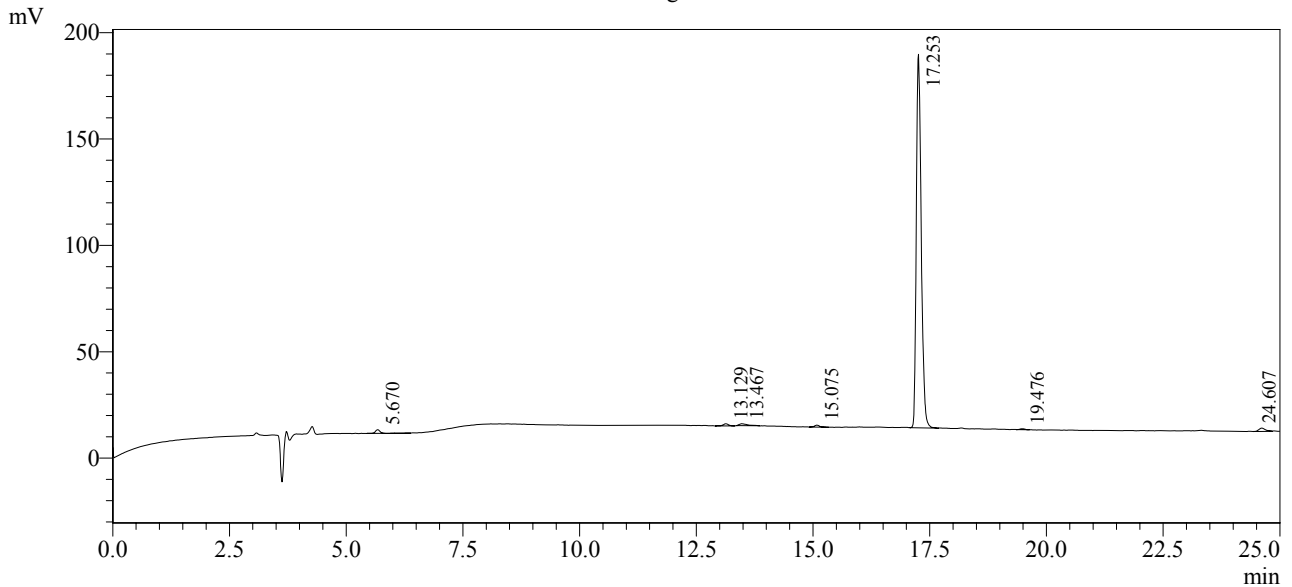

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	5.670	10819	1704	0.804
2	13.129	8328	1015	0.619
3	13.467	10978	892	0.815
4	15.075	7125	924	0.529
5	17.253	1289879	175612	95.822
6	19.476	2872	428	0.213
7	24.607	16120	1577	1.197
Total		1346119	182153	100.000