


Mass Spectrum

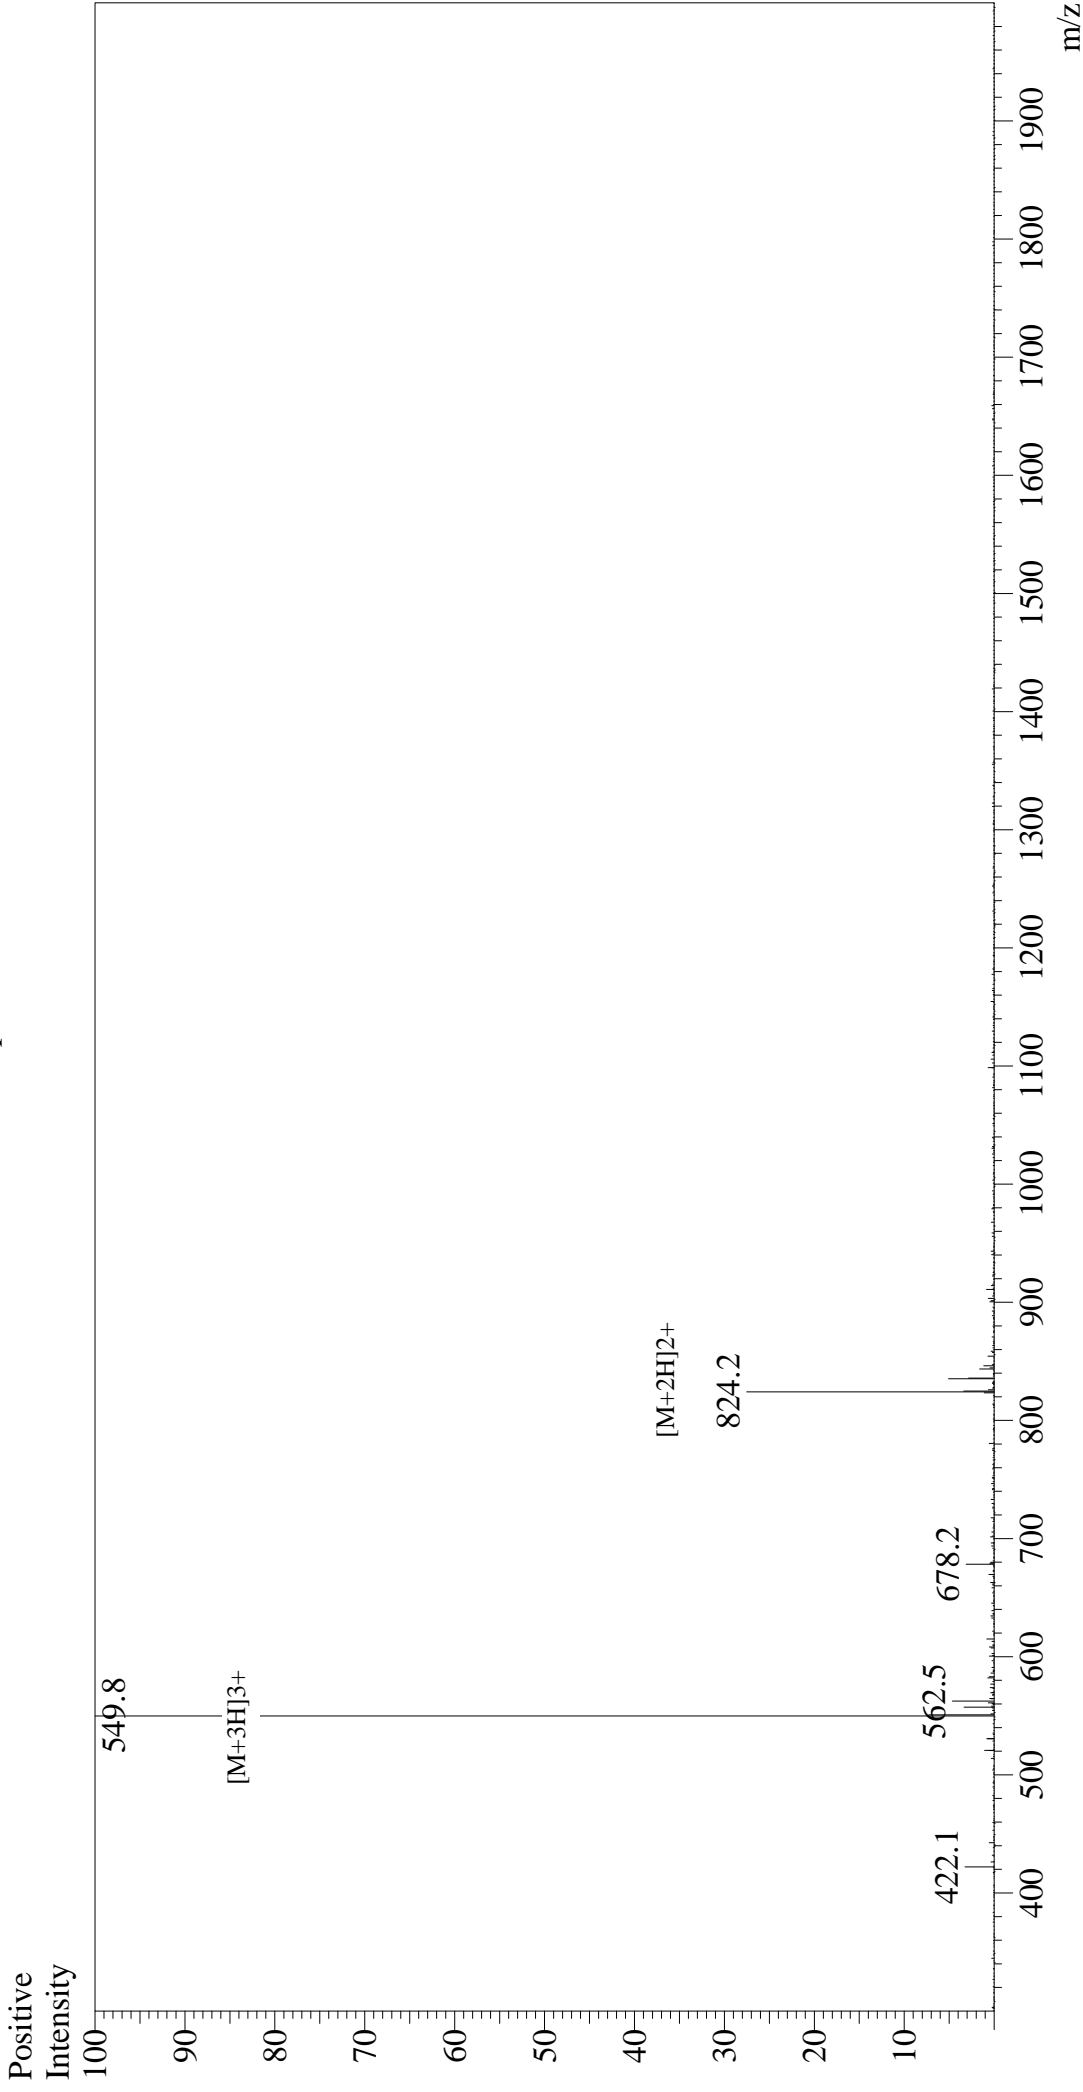

Sample Information

Acquired by : Gary
Month-Day Processed : 01/14/20
Time Processed : 21:20:18
Injection Volume : 0.4
Sample Name : [Nle4, D-Phe7]- α -Melanocyte Stimulating Hormone (MSH), amide
Cat. No. : RP10658
Lot. No. : E9734520A
Theoretical MW : 1647.00
Observed MW : 1646.4

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50% H₂O/50% MeOH