

Sample Name :HA Peptide  
 Cat. No. : RP11735  
 Lot. No. : PE7101710

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

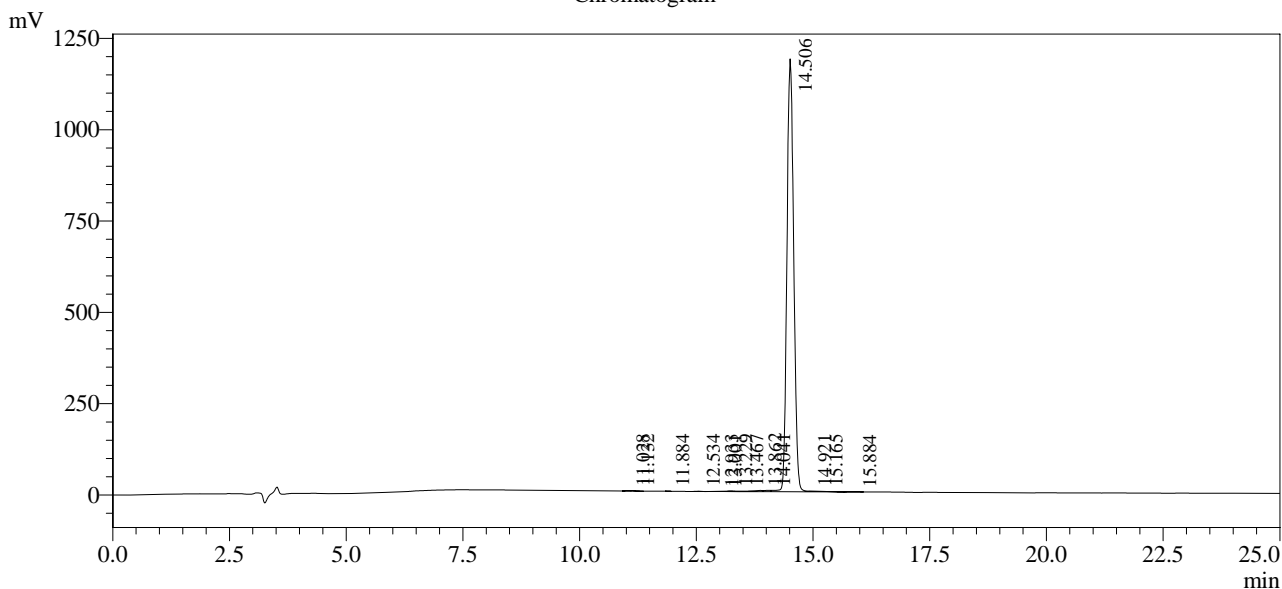

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.028	6229	872	0.051
2	11.132	6295	916	0.052
3	11.884	601	160	0.005
4	12.534	4627	640	0.038
5	12.933	4128	484	0.034
6	13.001	2571	528	0.021
7	13.229	30947	2207	0.253
8	13.467	5498	1112	0.045
9	13.862	58802	3462	0.482
10	14.041	35377	3737	0.290
11	14.506	12003855	1185193	98.301
12	14.921	21086	2097	0.173
13	15.165	24366	1810	0.200
14	15.884	6951	524	0.057
Total		12211334	1203742	100.000