

Sample Name:MDYKDHDGDYKDHDIDYKDDDDK peptide  
 Cat No. :RP21087  
 Lot No. :E8965021F  
 Time Processed :9:29:26 AM  
 Month-Day-Year Processed :06/19/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010141

<Chromatogram>

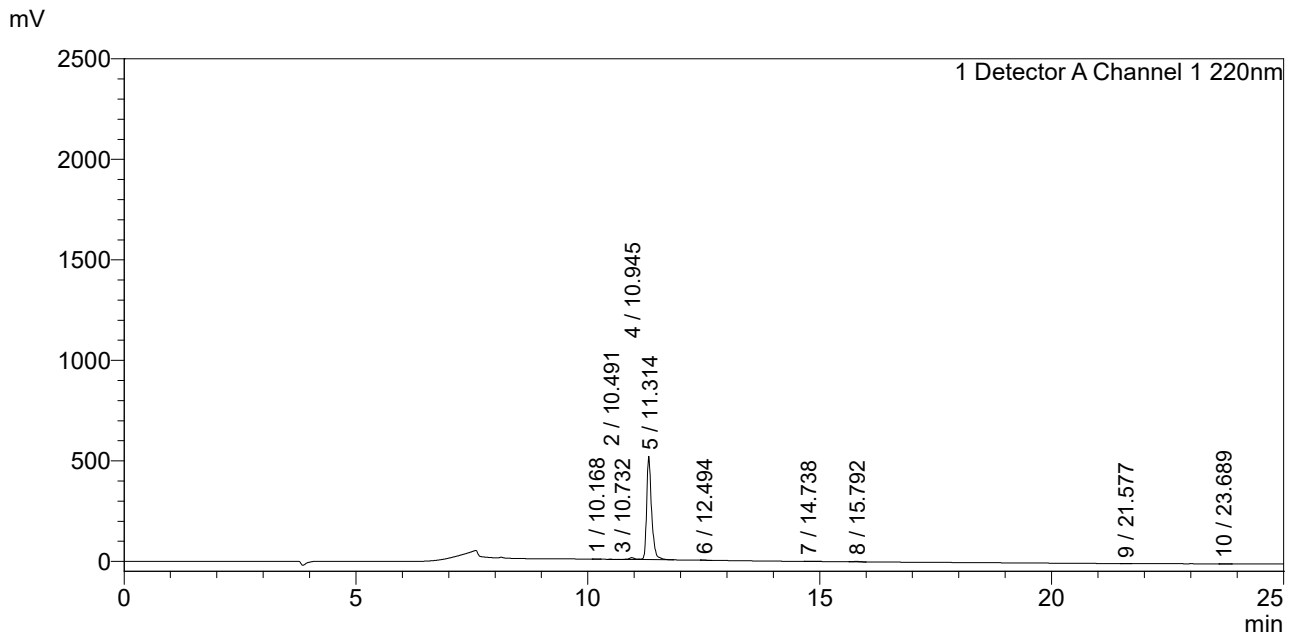

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.168	3034	624	0.077
2	10.491	2070	403	0.053
3	10.732	2686	585	0.068
4	10.945	79681	9402	2.032
5	11.314	3808239	513406	97.094
6	12.494	3223	444	0.082
7	14.738	4113	269	0.105
8	15.792	17159	2430	0.437
9	21.577	1011	140	0.026
10	23.689	1021	119	0.026
Total		3922237	527822	100.000