

Sample Name :Neuropeptide Y, human
 Cat No. :RP10492
 Lot No. :E7717121D
 Time Processed :9:20:16
 Month-Day-Year Processed :04/21/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

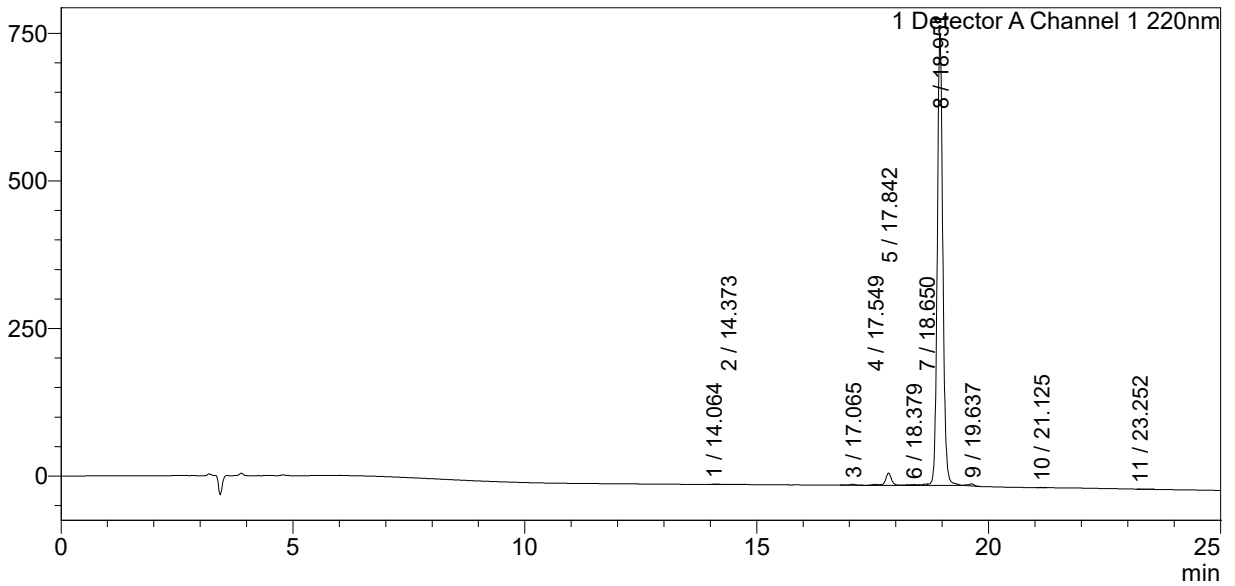

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.064	3950	261	0.059
2	14.373	5488	321	0.082
3	17.065	14779	1596	0.222
4	17.549	15577	1452	0.234
5	17.842	183533	20850	2.755
6	18.379	5601	680	0.084
7	18.650	16334	2305	0.245
8	18.951	6379654	765410	95.769
9	19.637	33406	3611	0.501
10	21.125	1466	247	0.022
11	23.252	1722	107	0.026
Total		6661512	796838	100.000