

Sample Name :β-Amyloid (1-42), human  
 Cat No. : RP10017  
 Lot No. : PE9781611

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	10
25.00	Pumps	Pump B Conc.	100
25.01	Pumps	Pump B Conc.	95
31.00	Pumps	Pump B Conc.	95
31.01	Pumps	Pump B Conc.	10
40.00	Pumps	Pump B Conc.	10
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Boston Green C4 4.6 x 250 mm

### <Chromatogram>

mV

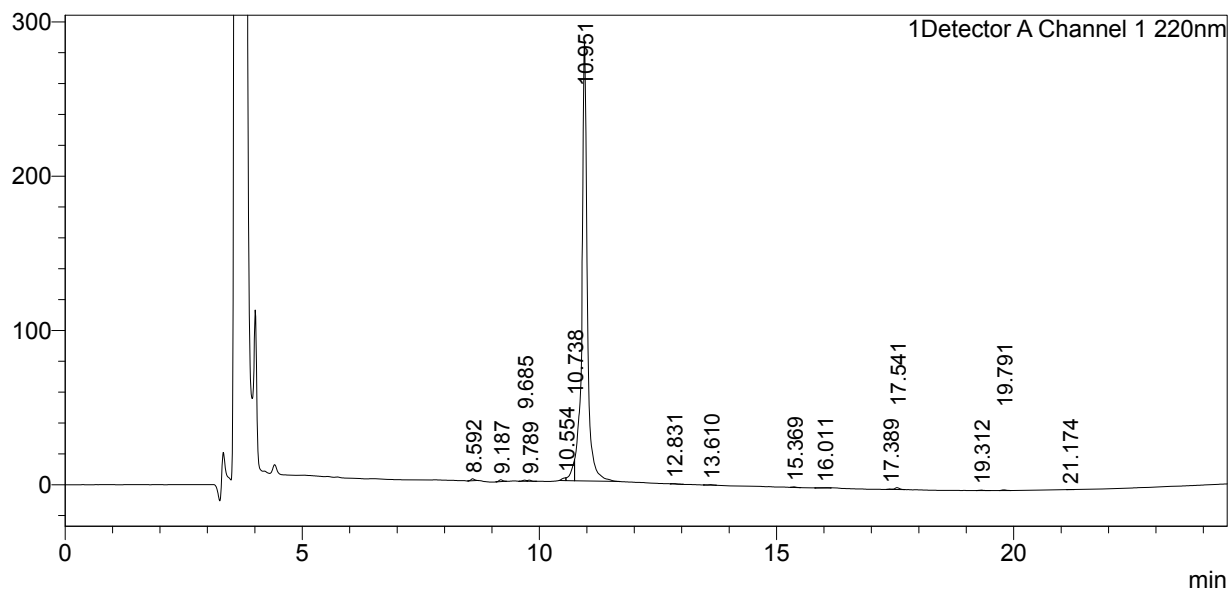

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.592	6423	1259	0.271
2	9.187	6388	1177	0.270
3	9.685	4154	756	0.175
4	9.789	3698	759	0.156
5	10.554	9624	1770	0.406
6	10.738	66156	12809	2.792
7	10.951	2251437	285227	95.014
8	12.831	950	211	0.040
9	13.610	2164	340	0.091
10	15.369	1728	346	0.073
11	16.011	2531	269	0.107
12	17.389	1376	279	0.058
13	17.541	7969	1219	0.336
14	19.312	1812	293	0.076
15	19.791	2455	423	0.104
16	21.174	719	150	0.030
Total		2369583	307288	100.000