

Sample Name :HA Peptide
 Cat No. : RP11735
 Lot No. : E0687421A
 Time Processed :7:23:54 AM
 Month-Day-Year Processed :01/27/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment:ZJ17010508

<Chromatogram>

mV

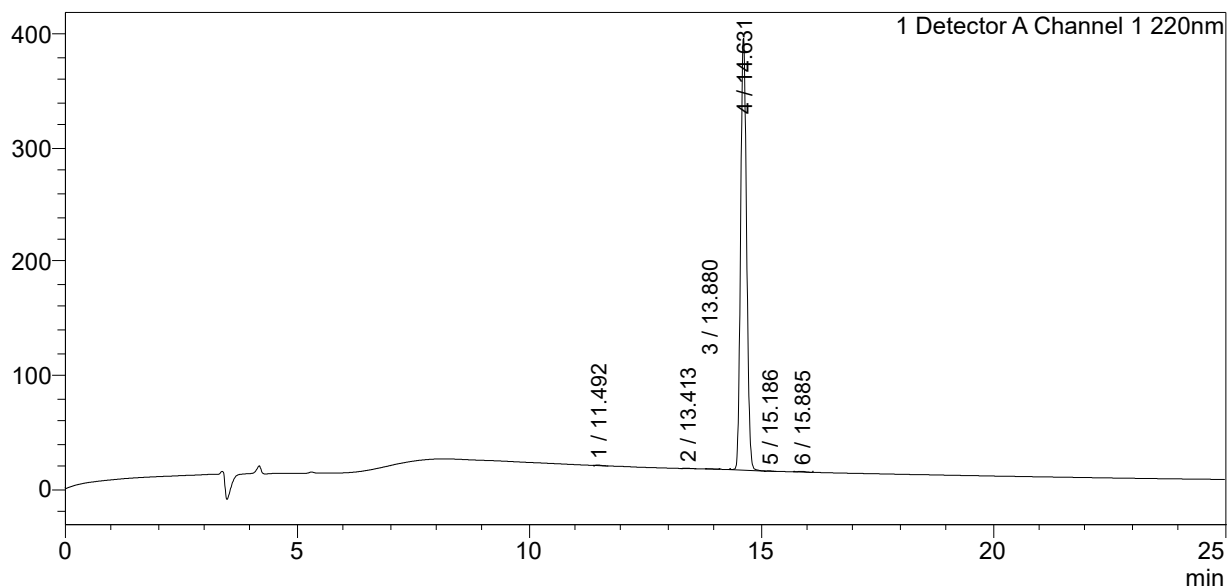

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.492	3315	460	0.096
2	13.413	3104	416	0.090
3	13.880	1012	114	0.029
4	14.631	3420963	380562	99.542
5	15.186	1485	255	0.043
6	15.885	6811	677	0.198
Total		3436689	382482	100.000