

Sample Name :HA Peptide
 Cat No :RP11735
 Lot No :E3764021B
 Time Processed :19:53:05
 Month-Day-Year Processed :02/05/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: SS-CM-0309

<Chromatogram>

mV

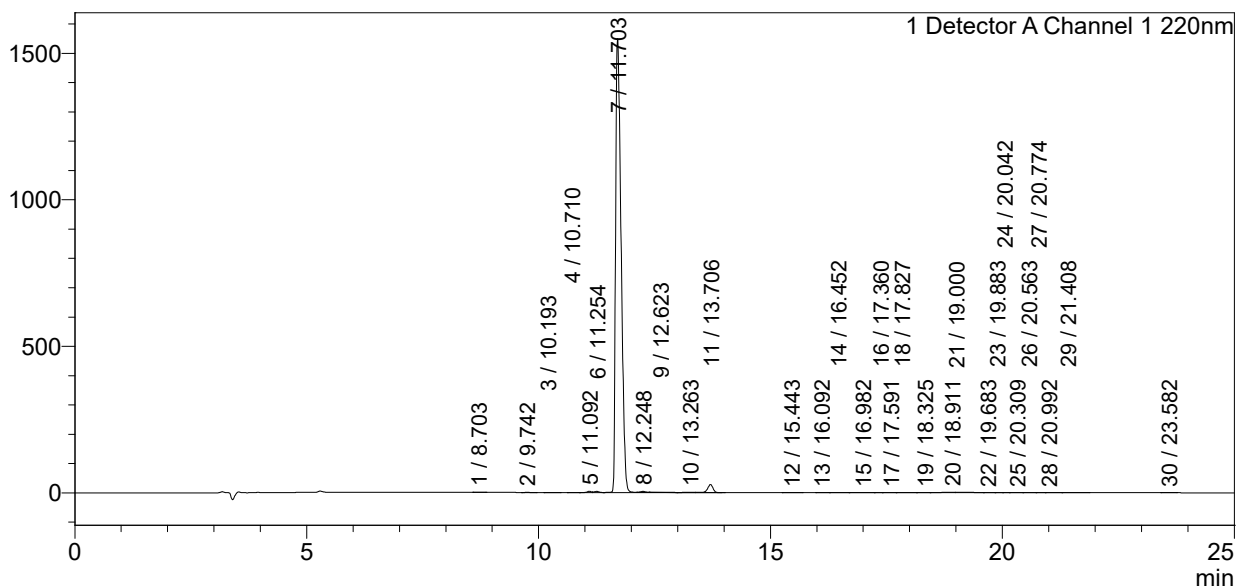

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.703	3149	498	0.024
2	9.742	1250	132	0.009
3	10.193	1625	158	0.012
4	10.710	1455	137	0.011
5	11.092	28616	4696	0.215
6	11.254	28344	3943	0.213
7	11.703	12832931	1549562	96.532
8	12.248	21317	3206	0.160
9	12.623	12614	701	0.095
10	13.263	8104	802	0.061
11	13.706	221764	27679	1.668
12	15.443	2235	155	0.017
13	16.092	1253	92	0.009
14	16.452	2380	136	0.018
15	16.982	8808	452	0.066
16	17.360	1914	211	0.014

Peak#	Ret. Time	Area	Height	Area%
17	17.591	4000	247	0.030
18	17.827	6374	301	0.048
19	18.325	3593	225	0.027
20	18.911	21355	988	0.161
21	19.000	27395	969	0.206
22	19.683	8530	595	0.064
23	19.883	5240	544	0.039
24	20.042	3972	507	0.030
25	20.309	7571	451	0.057
26	20.563	8199	572	0.062
27	20.774	4550	405	0.034
28	20.992	6290	362	0.047
29	21.408	6817	313	0.051
30	23.582	2355	300	0.018
Total		13293999	1599339	100.000