

Sample Name :HA Peptide  
 Cat No. :RP11735  
 Lot No. :PE8861901  
 Time Processed :10:13:44  
 Month-Day-Year Processed :01/18/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ17010508

<Chromatogram>

mV

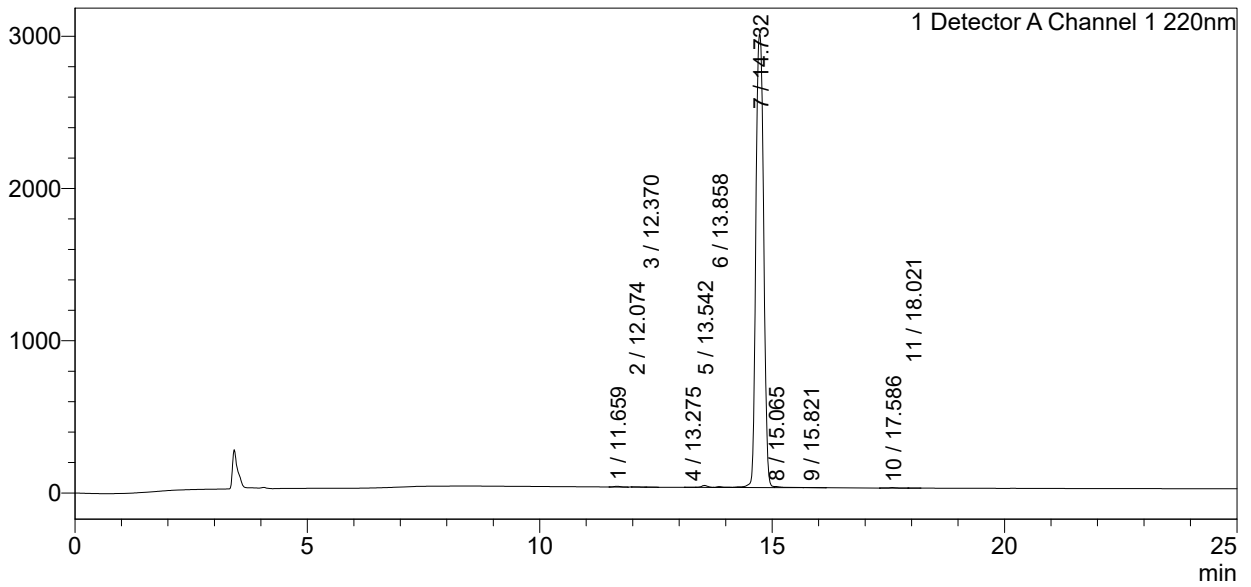

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.659	44657	4851	0.128
2	12.074	5213	645	0.015
3	12.370	3042	452	0.009
4	13.275	5369	543	0.015
5	13.542	116848	12585	0.335
6	13.858	60949	5461	0.175
7	14.732	34458320	2980496	98.928
8	15.065	78500	7129	0.225
9	15.821	25142	2200	0.072
10	17.586	30773	3404	0.088
11	18.021	2861	395	0.008
Total		34831673	3018162	100.000