

Sample Name : HA Peptide  
 Cat No.: RP11735  
 Lot No.: E2666621D  
 Time Processed :9:56:15  
 Month-Day-Year Processed :04/11/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010014

### <Chromatogram>

mV

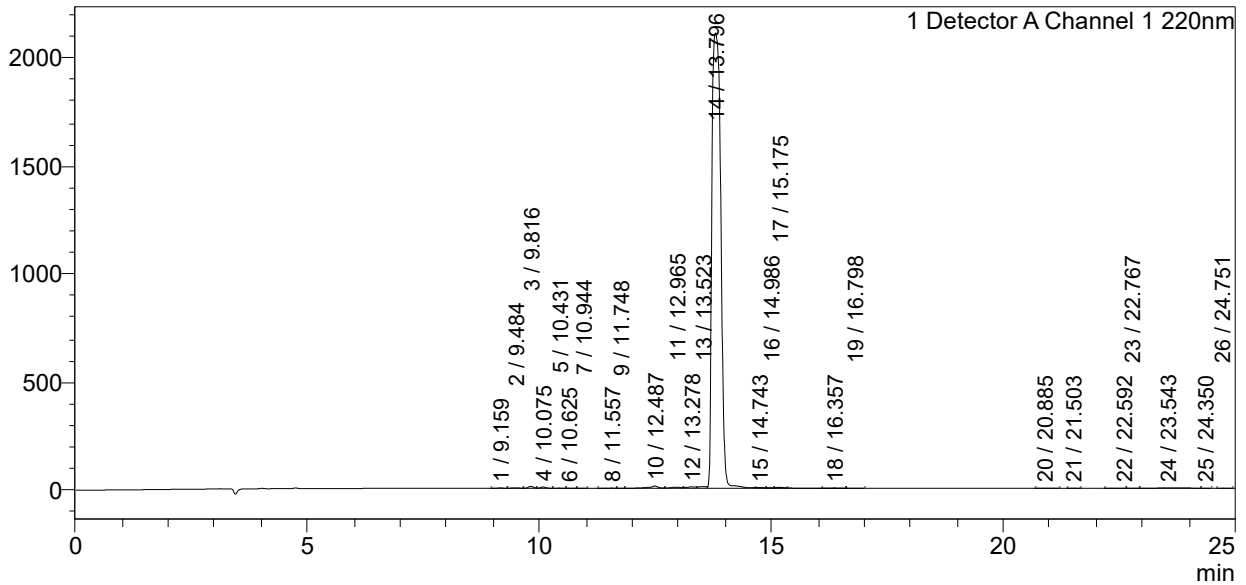

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.159	3870	573	0.014
2	9.484	14151	1747	0.049
3	9.816	61955	8885	0.216
4	10.075	39186	5509	0.137
5	10.431	3528	441	0.012
6	10.625	3304	372	0.012
7	10.944	2204	307	0.008
8	11.557	5082	553	0.018
9	11.748	1737	216	0.006
10	12.487	141974	9873	0.496
11	12.965	71894	4748	0.251
12	13.278	79808	6723	0.279
13	13.523	96046	7826	0.336
14	13.796	27991831	2107535	97.799
15	14.743	6766	927	0.024

Peak#	Ret. Time	Area	Height	Area%
16	14.986	4140	746	0.014
17	15.175	32797	3454	0.115
18	16.357	7124	615	0.025
19	16.798	4836	506	0.017
20	20.885	5566	359	0.019
21	21.503	1908	157	0.007
22	22.592	2468	214	0.009
23	22.767	1935	156	0.007
24	23.543	34409	868	0.120
25	24.350	1375	156	0.005
26	24.751	1909	222	0.007
Total		28621804	2163689	100.000