

Sample Name : [Nle4, D-Phe7]- $\alpha$ -MSH, amide  
 Cat. No. : RP10658-1  
 Lot. No. : PE6651709

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

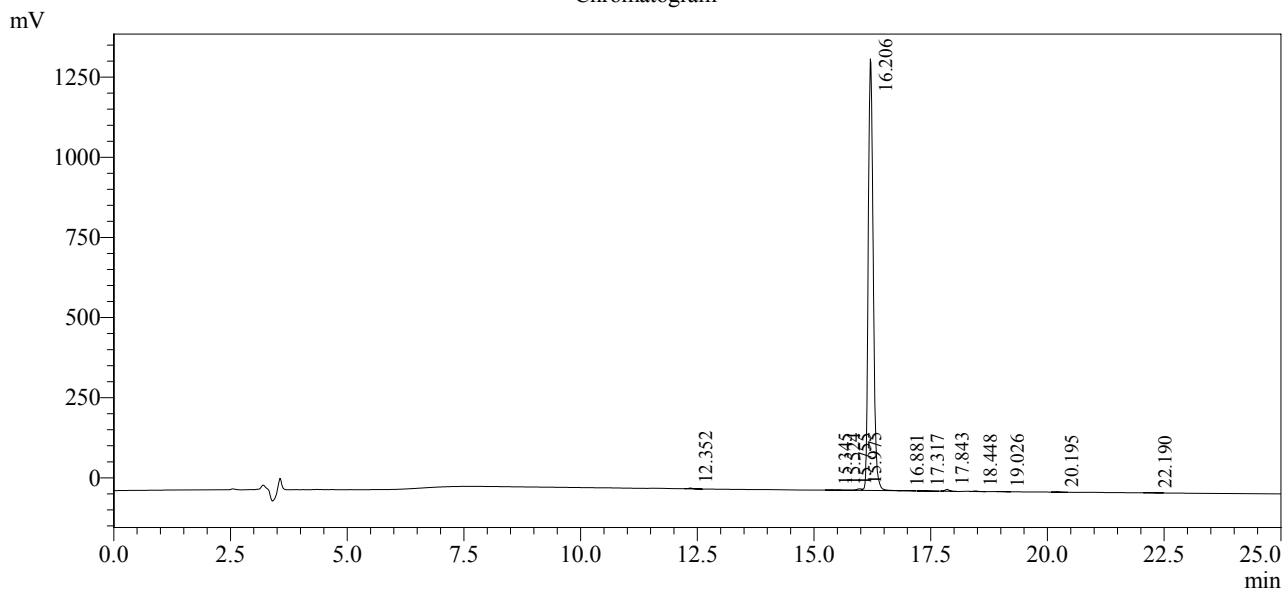

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.352	16177	2397	0.160
2	15.345	10763	1624	0.106
3	15.524	10830	1116	0.107
4	15.755	9017	985	0.089
5	15.975	39504	4836	0.391
6	16.206	9955288	1346520	98.431
7	16.881	4966	190	0.049
8	17.317	4571	494	0.045
9	17.843	36101	5724	0.357
10	18.448	11657	1764	0.115
11	19.026	5532	849	0.055
12	20.195	5279	779	0.052
13	22.190	4294	388	0.042
Total		10113978	1367665	100.000