

Sample Name : β -Amyloid (1-42), human
 Cat. No. : RP10017
 Lot. No.: PE5471812
 Time Processed : 14:21:55
 Month-Day-Year Processed : 01/24/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	10	
25.00	Pumps	Pump A B.Conc	100	
25.01	Pumps	Pump A B.Conc	95	
30.00	Pumps	Pump A B.Conc	95	
30.01	Pumps	Pump A B.Conc	10	
35.00	Pumps	Pump A B.Conc	10	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

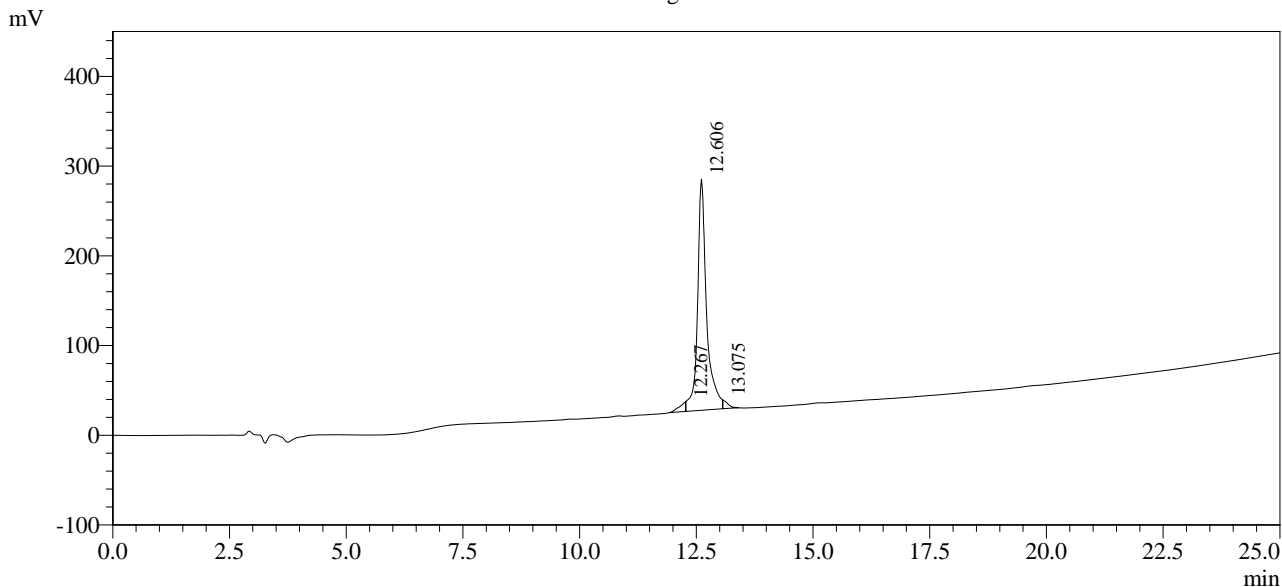

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.267	103400	10936	2.846
2	12.606	3461284	257610	95.257
3	13.075	68953	9616	1.898
Total		3633638	278162	100.000