

Sample Name :HA Peptide
 Cat No. : RP11735
 Lot No. : E7291519L
 Time Processed : 16:22:11
 Month-Day-Year Processed : 12/13/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment:GK12010012

<Chromatogram>

mV

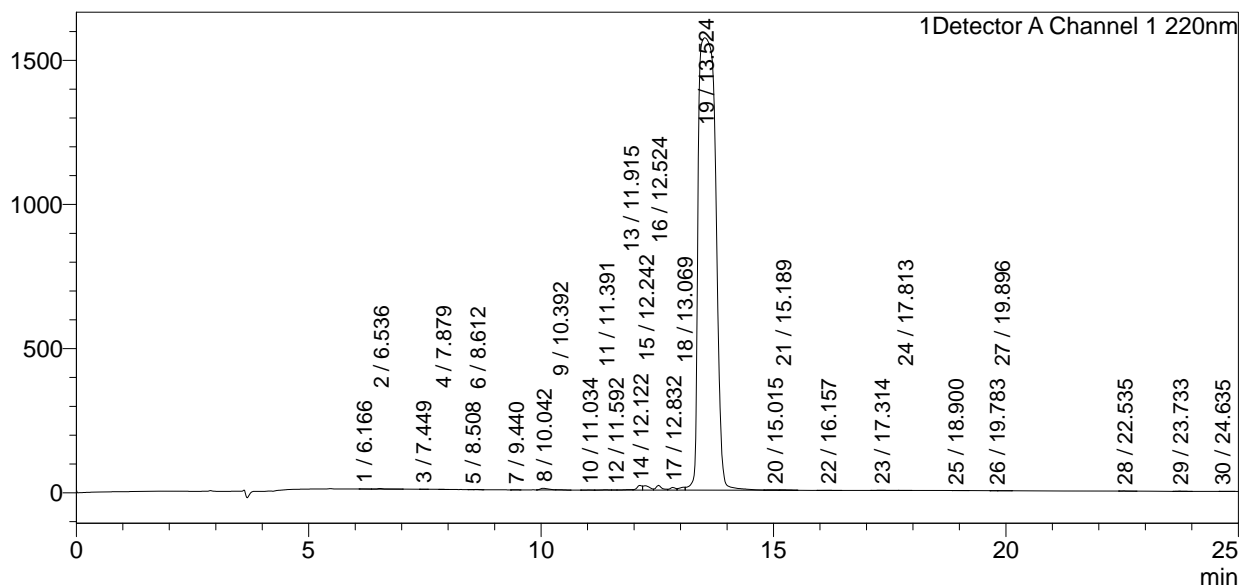

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	6.166	1910	150	0.005
2	6.536	20218	2265	0.049
3	7.449	1237	248	0.003
4	7.879	2008	415	0.005
5	8.508	1393	294	0.003
6	8.612	4606	730	0.011
7	9.440	2630	410	0.006
8	10.042	71649	5681	0.173
9	10.392	9834	1043	0.024
10	11.034	4317	436	0.010
11	11.391	13937	1175	0.034
12	11.592	4832	729	0.012
13	11.915	27114	1952	0.066
14	12.122	126712	16495	0.307
15	12.242	150595	15176	0.364

Peak#	Ret. Time	Area	Height	Area%
16	12.524	146406	16614	0.354
17	12.832	79017	9526	0.191
18	13.069	88132	10210	0.213
19	13.524	40515999	1568836	98.036
20	15.015	6431	536	0.016
21	15.189	7558	588	0.018
22	16.157	7434	585	0.018
23	17.314	10760	790	0.026
24	17.813	4466	703	0.011
25	18.900	1417	141	0.003
26	19.783	1239	200	0.003
27	19.896	3093	315	0.007
28	22.535	4928	591	0.012
29	23.733	6547	705	0.016
30	24.635	1415	111	0.003
Total		41327832	1657650	100.000