

Sample Name : hgp100(25-33)

Cat No.: RP20344 Lot No.: PE2451709

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow: 1 ml/min

Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
10.00	Pumps	Pump A B.Conc	35	
35.00	Pumps	Pump A B.Conc	95	
41.00	Pumps	Pump A B.Conc	95	
41.01	Pumps	Pump A B.Conc	5	
50.00	Pumps	Pump A B.Conc	5	
50.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

Chromatogram

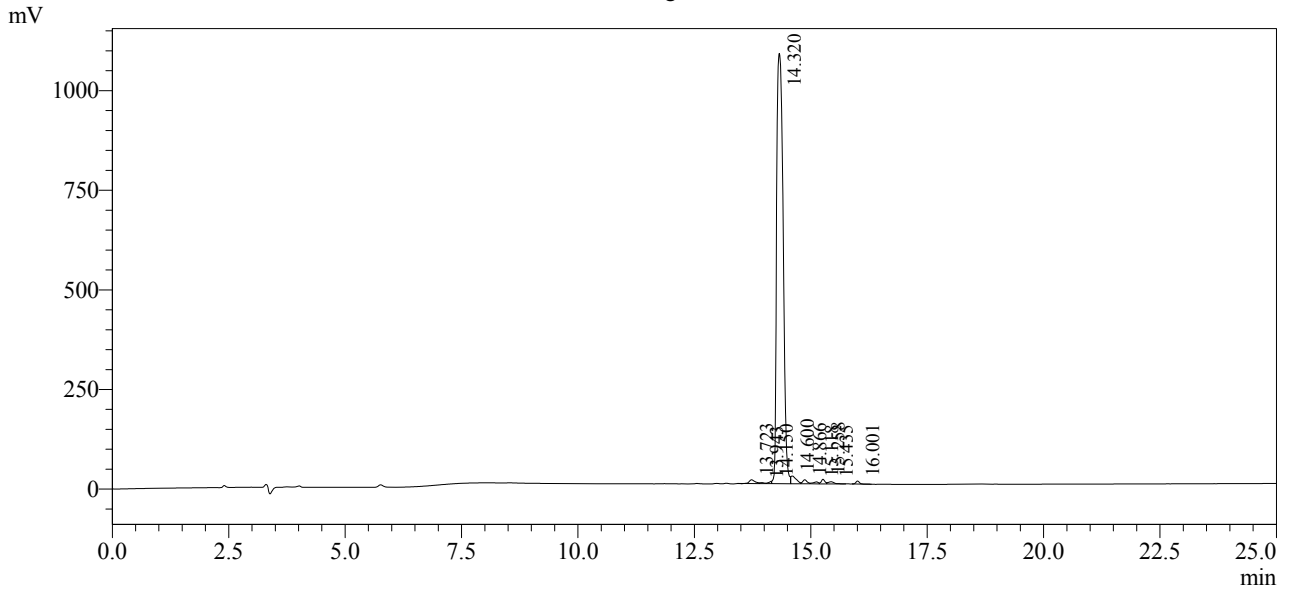

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.723	81434	9404	0.739
2	13.943	17120	2420	0.155
3	14.150	25056	5938	0.227
4	14.320	10486257	1079712	95.171
5	14.600	152889	19396	1.388
6	14.866	67236	10249	0.610
7	15.118	37822	4841	0.343
8	15.258	61429	11410	0.558
9	15.435	49392	5379	0.448
10	16.001	39680	7655	0.360
Total		11018314	1156403	100.000