

Sample Name :[Nle4, D-Phe7]- α -MSH, amide
 Cat. No. : RP10658
 Lot. No. : E5058420F
 Time Processed :8:13:42
 Month-Day-Year Processed :06/17/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment :SS-CM-0310

Chromatogram

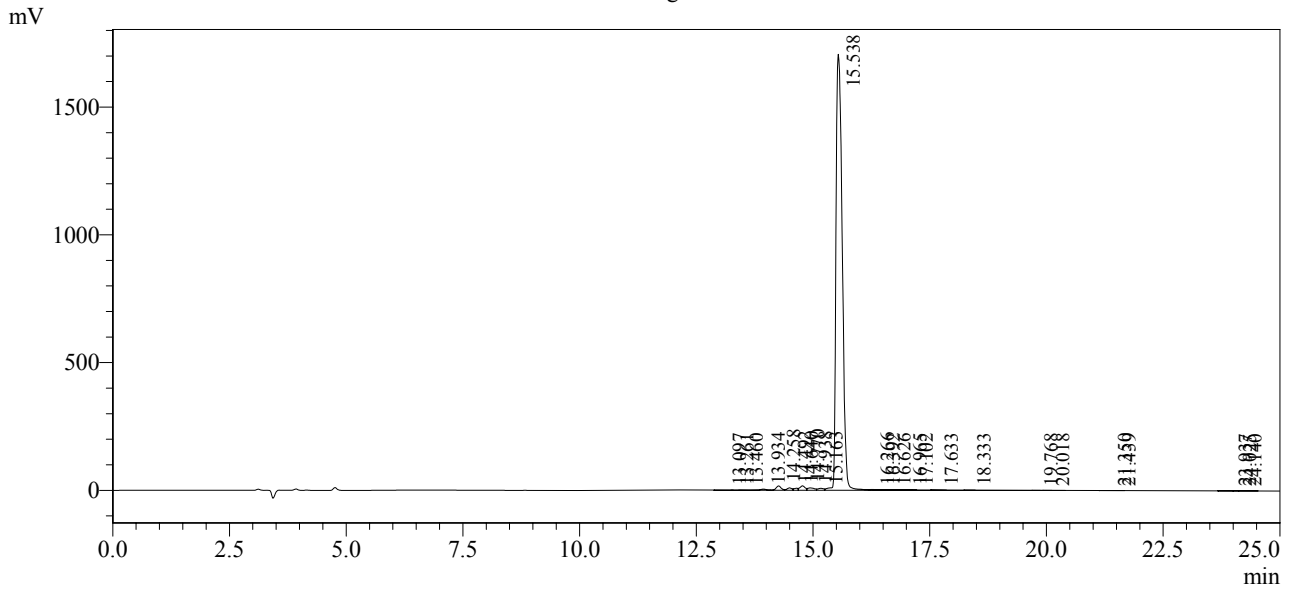

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.097	9136	1005	0.055
2	13.261	6437	839	0.039
3	13.460	16710	1210	0.101
4	13.934	46938	4390	0.283
5	14.258	129851	17017	0.782
6	14.492	69117	9171	0.416
7	14.640	46308	7899	0.279
8	14.770	132028	17379	0.795
9	14.938	93676	9231	0.564
10	15.163	67003	7835	0.403
11	15.538	15945909	1706604	95.974
12	16.266	6533	1022	0.039
13	16.392	2227	498	0.013
14	16.626	7007	1213	0.042
15	16.965	5227	516	0.031
16	17.102	1635	289	0.010
17	17.633	7941	1168	0.048
18	18.333	1058	151	0.006
19	19.768	1362	160	0.008
20	20.018	1085	137	0.007
21	21.350	3427	350	0.021
22	21.439	3197	383	0.019
23	23.937	4035	330	0.024
24	24.025	1931	277	0.012

Peak#	Ret. Time	Area	Height	Area %
25	24.140	5003	310	0.030
Total		16614781	1789384	100.000