

Sample Name :HA Peptide
 Cat No. :RP11735
 Lot No. :E0685321A
 Time Processed :8:34:48 AM
 Month-Day-Year Processed :01/27/21

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

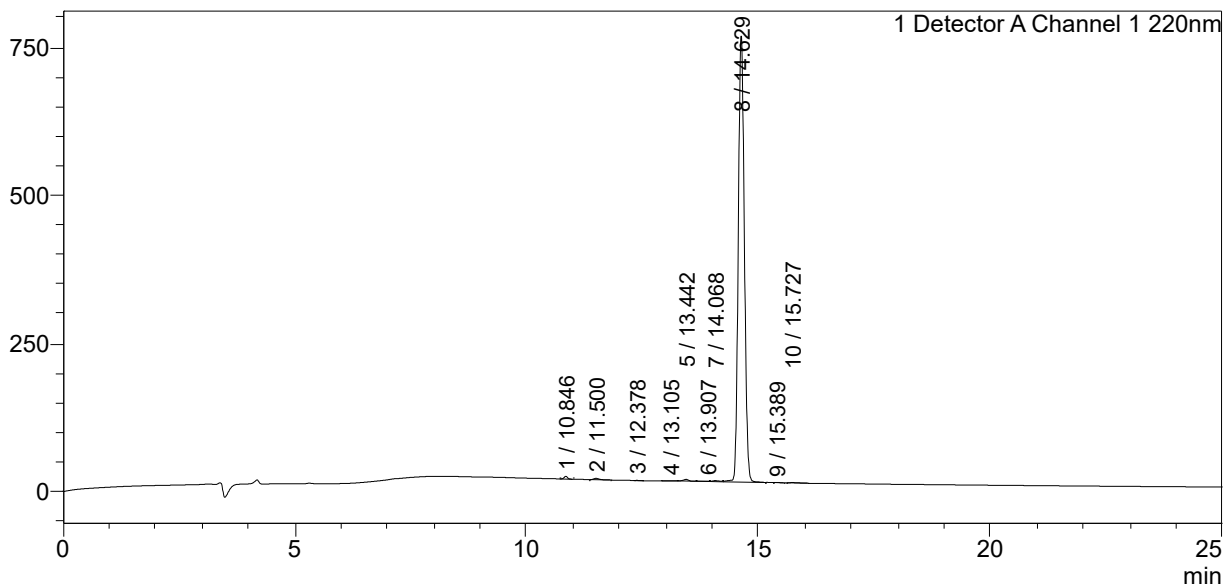

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.846	23166	4454	0.334
2	11.500	18380	2345	0.265
3	12.378	1913	349	0.028
4	13.105	1707	188	0.025
5	13.442	23749	3016	0.342
6	13.907	5628	591	0.081
7	14.068	19092	1720	0.275
8	14.629	6834904	752709	98.485
9	15.389	2034	268	0.029
10	15.727	9462	836	0.136
Total		6940036	766476	100.000