

Sample Name :HA Peptide
 Cat No. :RP11735
 Lot No. :E8193021C
 Time Processed :10:19:03
 Month-Day-Year Processed :03/14/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm
 <<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

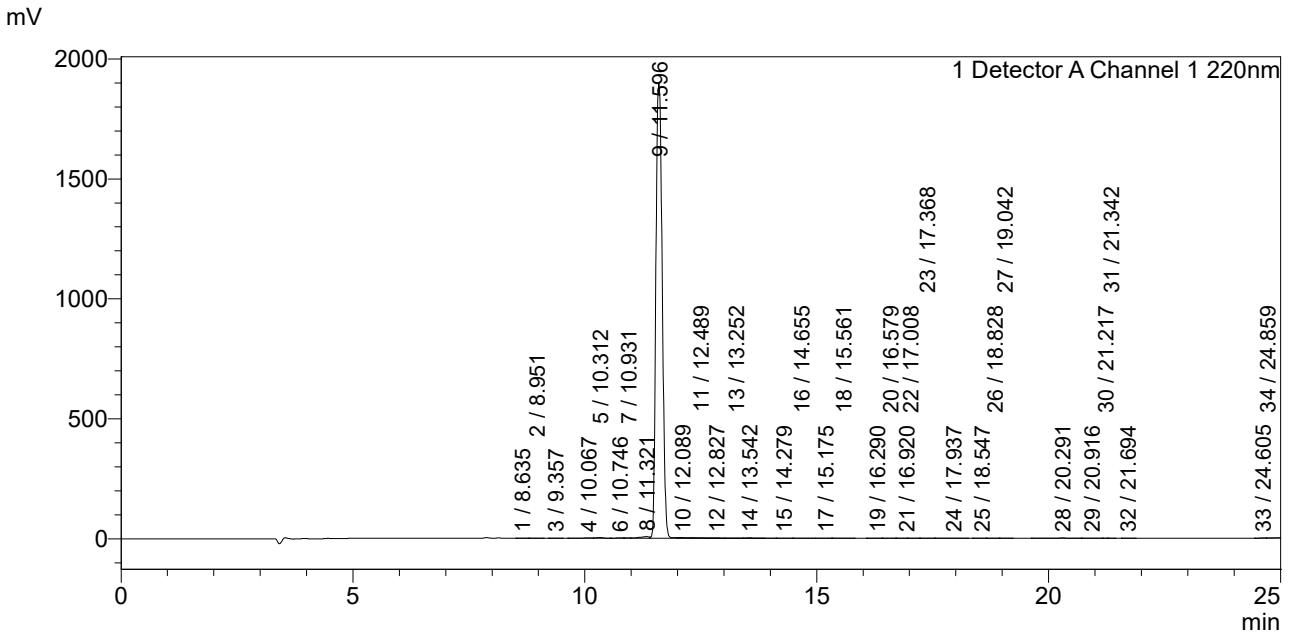

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.635	1954	256	0.011
2	8.951	1369	173	0.007
3	9.357	3897	448	0.021
4	10.067	33959	2017	0.186
5	10.312	42306	3789	0.232
6	10.746	20172	1791	0.110
7	10.931	13959	1735	0.076
8	11.321	111081	7127	0.608
9	11.596	17883147	1899434	97.949
10	12.089	8584	902	0.047
11	12.489	12562	1303	0.069
12	12.827	15968	1422	0.087
13	13.252	2959	272	0.016
14	13.542	17452	2150	0.096

Peak#	Ret. Time	Area	Height	Area%
15	14.279	5958	571	0.033
16	14.655	3849	311	0.021
17	15.175	1917	143	0.010
18	15.561	3035	152	0.017
19	16.290	2006	151	0.011
20	16.579	3344	278	0.018
21	16.920	2001	177	0.011
22	17.008	1680	159	0.009
23	17.368	1379	112	0.008
24	17.937	10614	502	0.058
25	18.547	1990	171	0.011
26	18.828	1945	144	0.011
27	19.042	1294	107	0.007
28	20.291	29250	835	0.160
29	20.916	8940	447	0.049
30	21.217	1210	193	0.007
31	21.342	1485	158	0.008
32	21.694	2475	199	0.014
33	24.605	2021	216	0.011
34	24.859	1937	148	0.011
Total		18257700	1927990	100.000