

Sample Name: HA Peptide
 Cat No. :RP11735
 Lot No. : E6875120H
 Time Processed: 9:25:43 AM
 Month-Day-Year Processed :08/06/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment:ZJ19010325

<Chromatogram>

mV

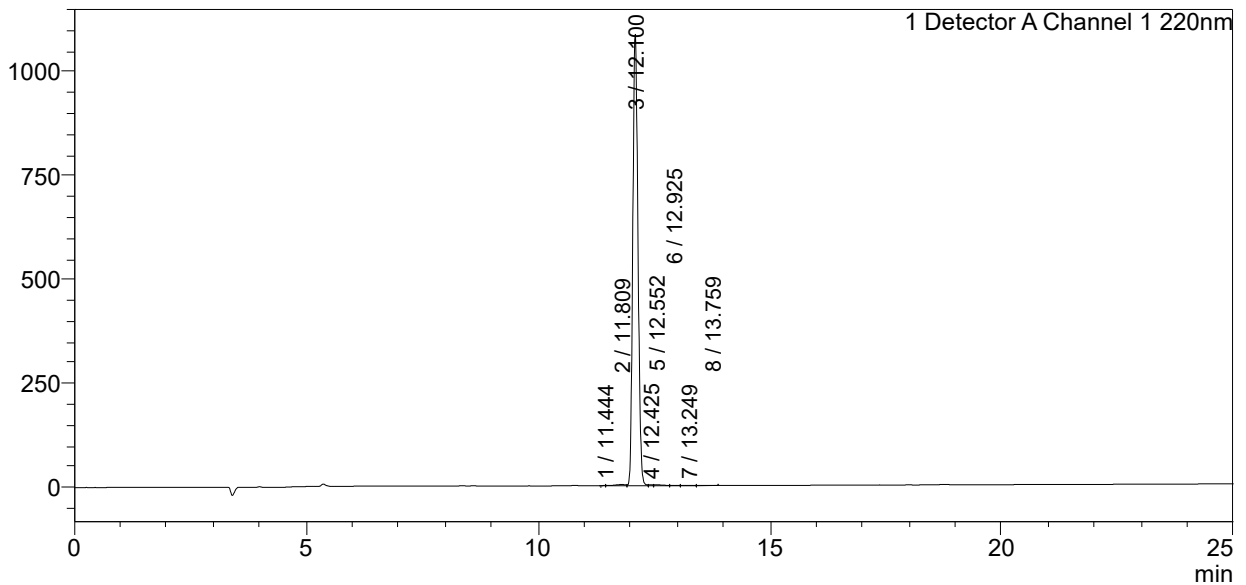

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.444	4955	743	0.058
2	11.809	52442	3415	0.612
3	12.100	8444637	1087346	98.500
4	12.425	12568	2302	0.147
5	12.552	36645	2487	0.427
6	12.925	8973	860	0.105
7	13.249	8495	716	0.099
8	13.759	4509	205	0.053
Total		8573224	1098074	100.000