

Sample Name : [Nle4, D-Phe7]- $\alpha$ -MSH, amide  
 Cat. No. : RP10658  
 Lot. No. : E6792819J  
 Time Processed : 8:39:39  
 Month-Day-Year Processed : 10/16/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: SS-CM-0286

Chromatogram

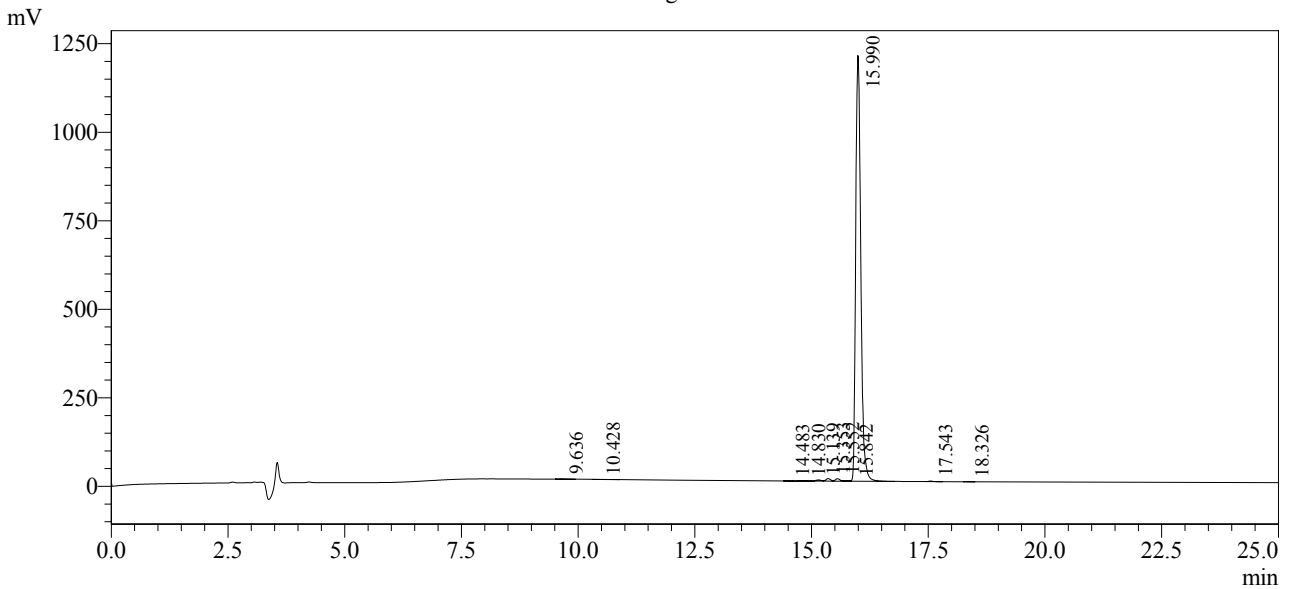

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.636	5779	716	0.062
2	10.428	4102	280	0.044
3	14.483	1123	210	0.012
4	14.830	6076	549	0.065
5	15.139	27191	3517	0.292
6	15.353	50078	7310	0.537
7	15.552	47082	7031	0.505
8	15.842	12108	1609	0.130
9	15.990	9153527	1202507	98.230
10	17.543	9822	1571	0.105
11	18.326	1620	238	0.017
Total		9318509	1225536	100.000