

Sample Name :MDYKDHDGDYKDHDIDYKDDDDK peptide
 Cat No. : RP21087
 Lot No. :E6127720G
 Time Processed : 17:34:13
 Month-Day-Year Processed : 07/12/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	55
25.10	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	95
50.00	Pumps	Pump A B.Conc	15
51.00	Pumps	Pump A B.Conc	15
95.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment:GK12010012

<Chromatogram>

mV

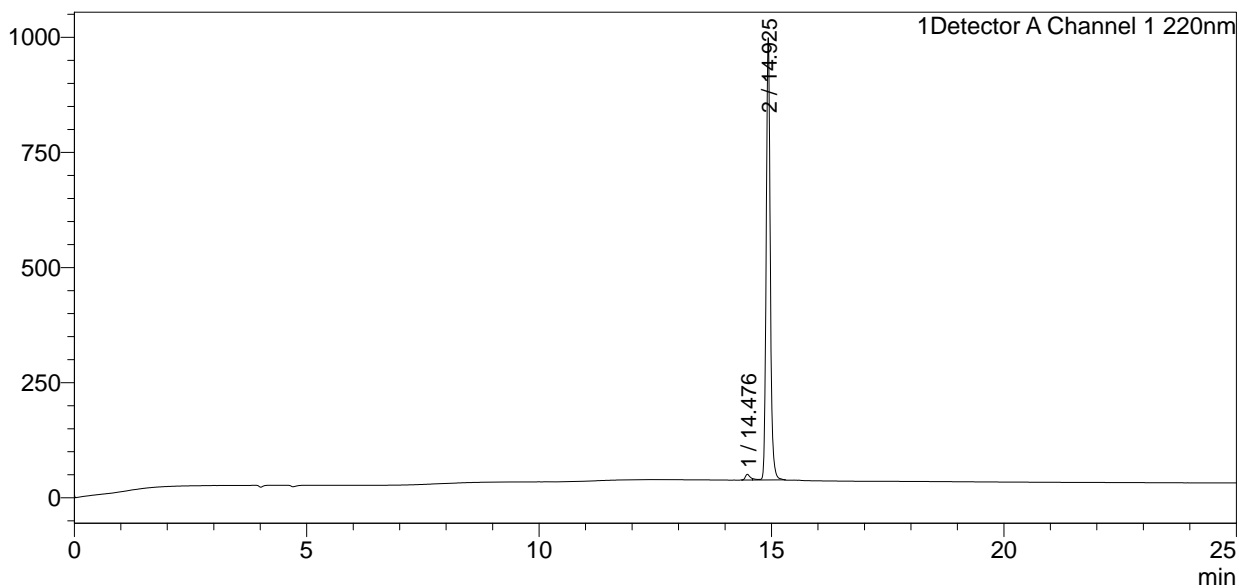

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.476	87276	12536	1.461
2	14.925	5884728	960006	98.539
Total		5972004	972542	100.000