

Sample Name : [Nle4, D-Phe7]- α -MSH, amide
 Cat. No. : RP10658
 Lot. No. : PE9411806

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

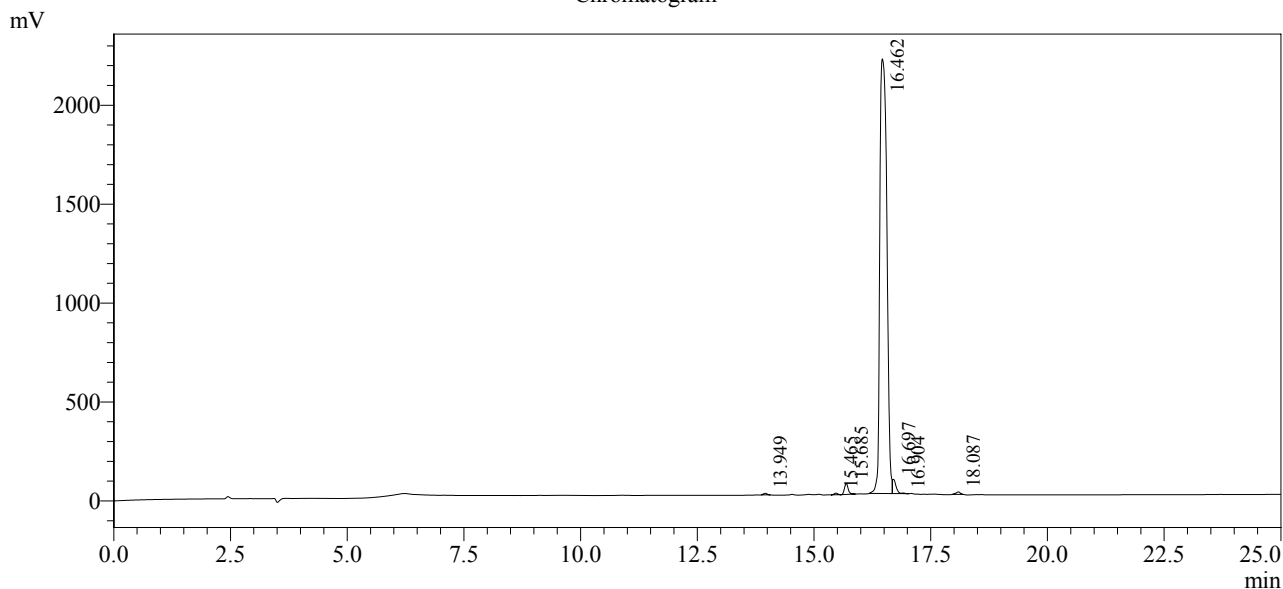

1 Det. A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.949	41711	7833	0.174
2	15.465	44107	8471	0.184
3	15.685	309757	56169	1.295
4	16.462	23063165	2197222	96.415
5	16.697	365706	72042	1.529
6	16.904	16358	3516	0.068
7	18.087	79906	12957	0.334
Total		23920710	2358210	100.000