

Sample Name :C-Peptide (3-33), human
 Cat. No. : RP11116
 Lot. No. : PE2011905
 Time Processed : 14:13:58
 Month-Day-Year Processed : 06/04/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	15	
25.00	Pumps	Pump A B.Conc	75	
25.01	Pumps	Pump A B.Conc	95	
30.00	Pumps	Pump A B.Conc	95	
30.01	Pumps	Pump A B.Conc	15	
40.00	Pumps	Pump A B.Conc	15	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

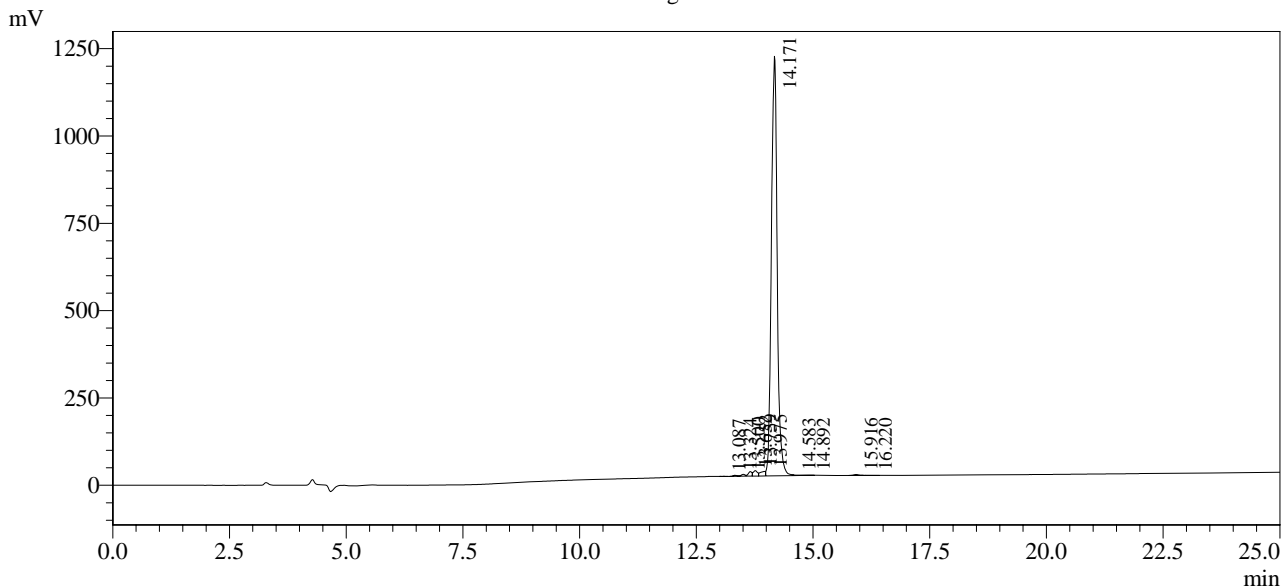

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.087	1504	321	0.014
2	13.324	17060	2776	0.159
3	13.500	31691	5314	0.295
4	13.652	71143	12946	0.663
5	13.759	97069	15483	0.904
6	13.975	102235	12944	0.952
7	14.171	10369985	1201240	96.610
8	14.583	13676	1880	0.127
9	14.892	11587	1275	0.108
10	15.916	14776	2107	0.138
11	16.220	3176	496	0.030
Total		10733902	1256781	100.000