

Sample Name :HA Peptide  
 Cat. No. : RP11735  
 Lot. No. : PE9641904  
 Time Processed : 14:48:50  
 Month-Day-Year Processed : 04/23/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	15	
25.00	Pumps	Pump A B.Conc	75	
25.01	Pumps	Pump A B.Conc	95	
30.00	Pumps	Pump A B.Conc	95	
30.01	Pumps	Pump A B.Conc	15	
40.00	Pumps	Pump A B.Conc	15	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

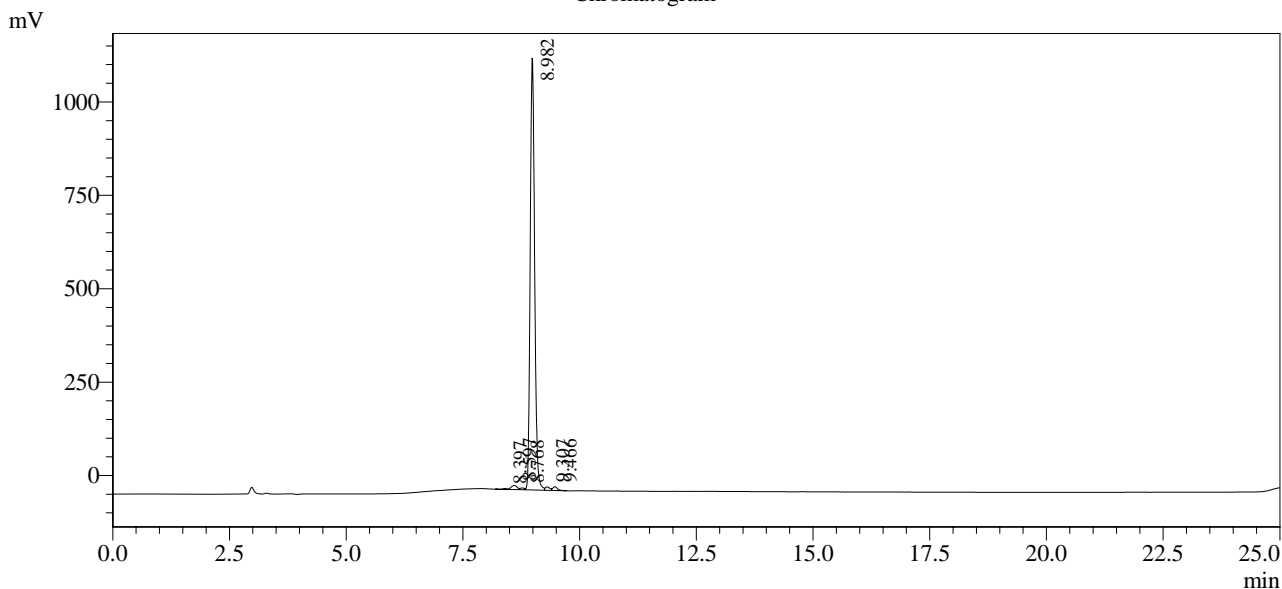

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.397	11456	1990	0.145
2	8.597	96604	11119	1.224
3	8.768	31069	4950	0.394
4	8.982	7620432	1155687	96.592
5	9.307	61958	9209	0.785
6	9.466	67795	10109	0.859
Total		7889314	1193064	100.000