

Sample Name : C-Peptide (3-33), human
 Cat. No. : RP11116
 Lot. No. : PE8021810
 Time Processed : 9:35:23
 Month-Day-Year Processed : 10/19/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010017

Chromatogram

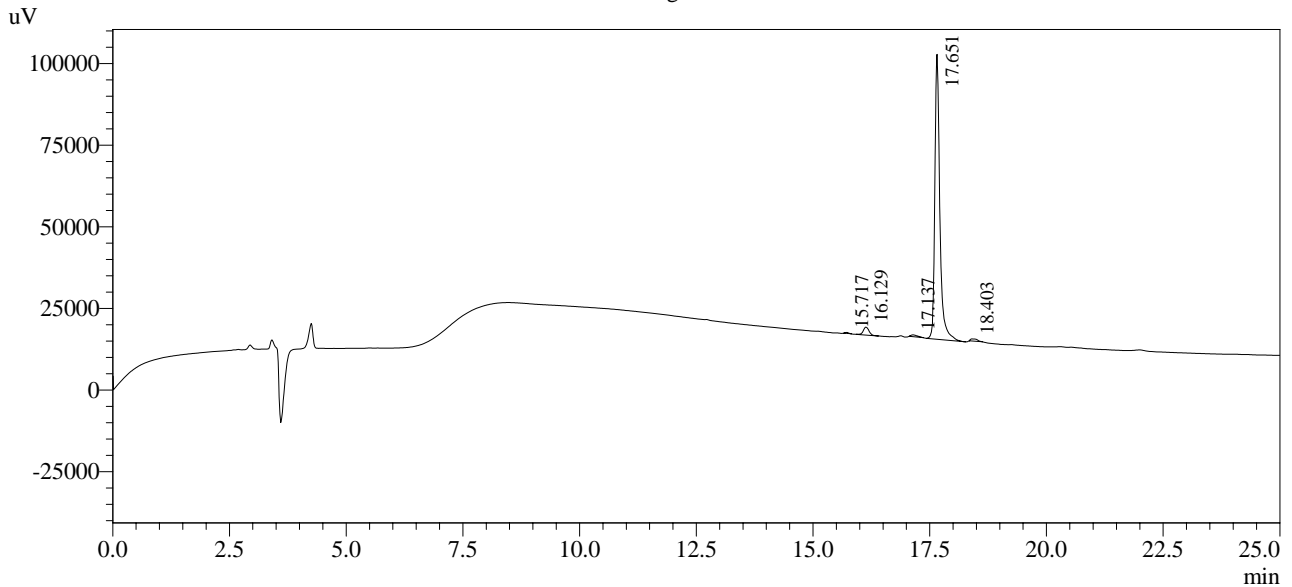

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.717	1405	285	0.205
2	16.129	20331	2400	2.970
3	17.137	5441	553	0.795
4	17.651	650895	87322	95.075
5	18.403	6542	623	0.956
Total		684614	91183	100.000