

Sample Name : β -Amyloid (25-35)
 Cat No. : RP10008
 Lot No. : E5845320F
 Time Processed : 8:50:19
 Month-Day-Year Processed : 06/03/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010140

<Chromatogram>

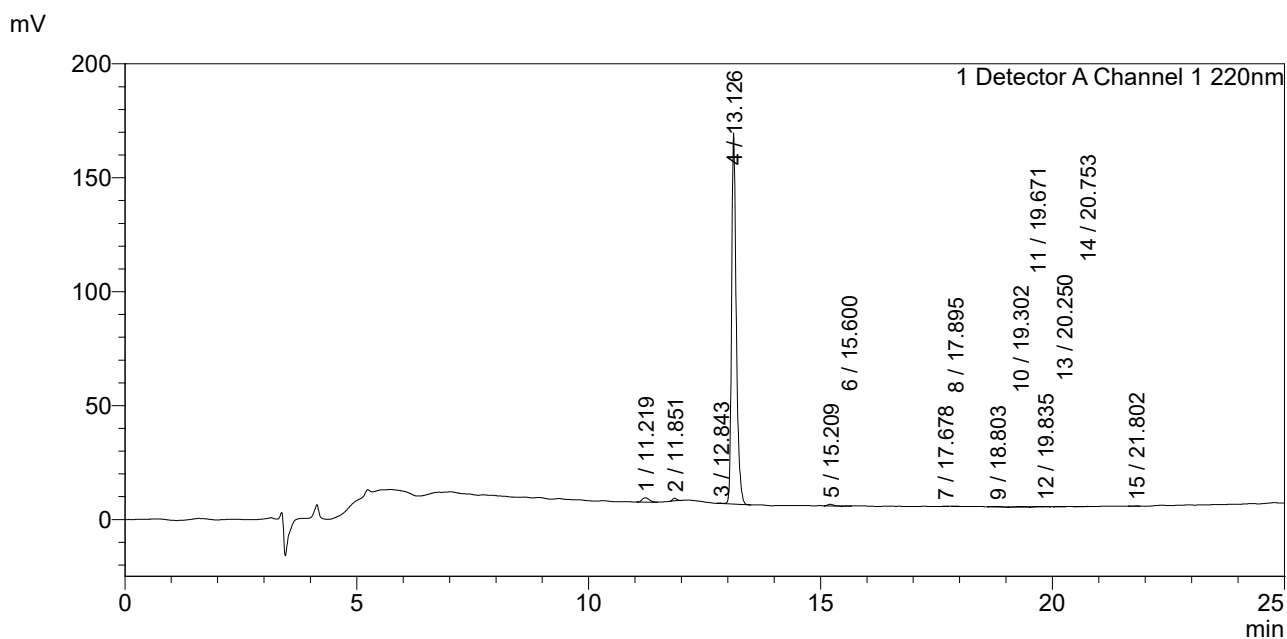

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.219	22477	1960	1.870
2	11.851	7017	1205	0.584
3	12.843	1285	184	0.107
4	13.126	1143644	162914	95.135
5	15.209	6445	722	0.536
6	15.600	1098	130	0.091
7	17.678	1460	167	0.121
8	17.895	2161	204	0.180
9	18.803	3067	224	0.255
10	19.302	4759	246	0.396
11	19.671	2653	205	0.221
12	19.835	1523	168	0.127
13	20.250	1620	126	0.135
14	20.753	1840	111	0.153
15	21.802	1080	96	0.090

Peak#	Ret. Time	Area	Height	Area%
Total		1202129	168662	100.000