

Sample Name : [Nle4, D-Phe7]- $\alpha$ -MSH, amide  
 Cat. No. : RP10658  
 Lot. No. : E47616191  
 Time Processed : 7:28:01  
 Month-Day-Year Processed : 09/22/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment : SS-CM-0310

Chromatogram

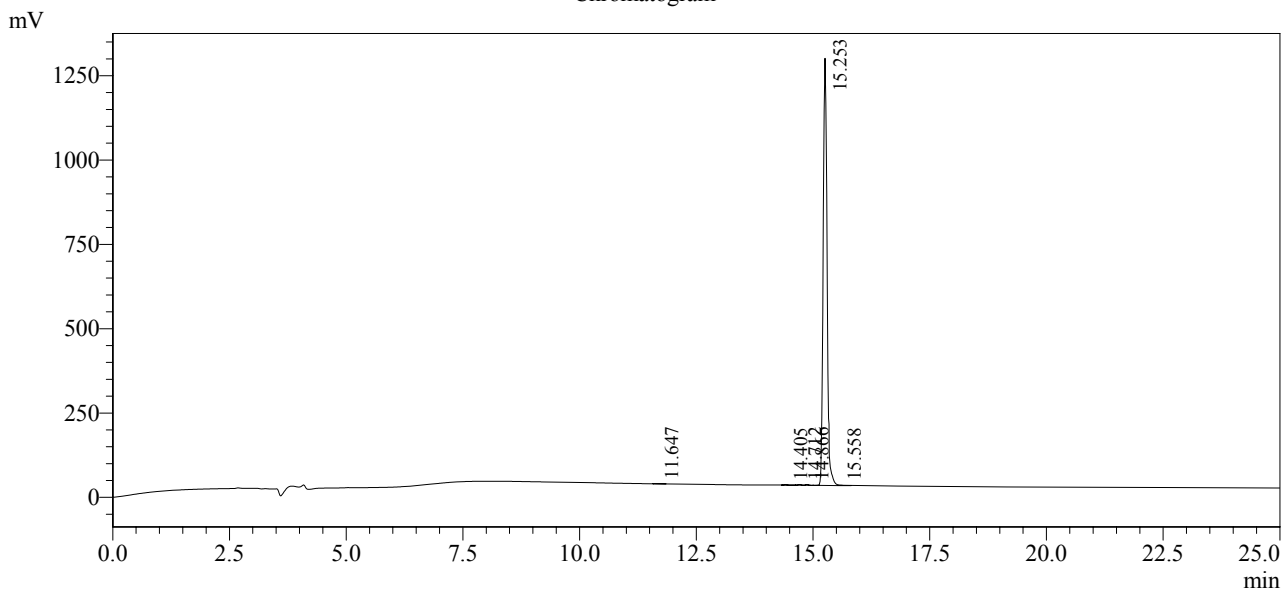

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.647	3337	517	0.045
2	14.405	6883	1268	0.092
3	14.712	12410	2296	0.166
4	14.866	12839	2570	0.172
5	15.253	7417321	1266526	99.377
6	15.558	11011	1544	0.148
Total		7463801	1274720	100.000