

Sample Name :HA Peptide
 Cat No. :RP11735
 Lot No. :E4919220K
 Time Processed :0:22:54
 Month-Day-Year Processed :11/18/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

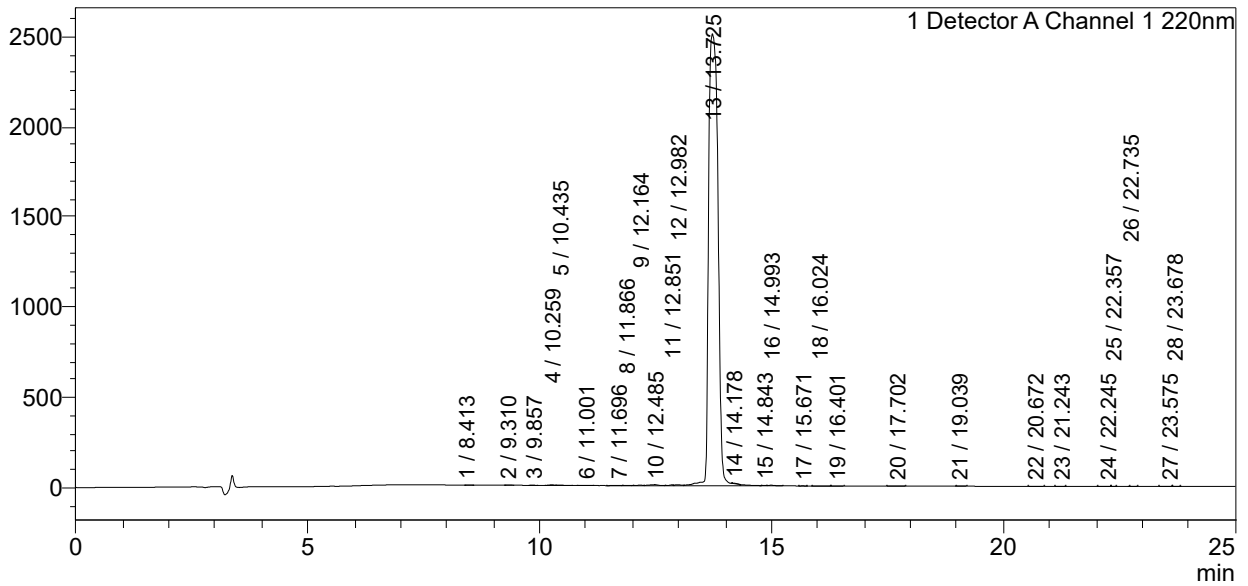

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.413	1244	144	0.004
2	9.310	1610	349	0.005
3	9.857	1662	262	0.005
4	10.259	23021	2929	0.065
5	10.435	17876	2464	0.051
6	11.001	7106	813	0.020
7	11.696	8427	986	0.024
8	11.866	9392	881	0.027
9	12.164	25025	2422	0.071
10	12.485	73306	5486	0.207
11	12.851	26214	4167	0.074
12	12.982	42667	3969	0.121
13	13.725	35014277	2503171	99.097
14	14.178	20907	2831	0.059

Peak#	Ret. Time	Area	Height	Area%
15	14.843	6606	1216	0.019
16	14.993	23769	3091	0.067
17	15.671	2027	428	0.006
18	16.024	4422	474	0.013
19	16.401	2326	265	0.007
20	17.702	8901	885	0.025
21	19.039	1015	131	0.003
22	20.672	1326	192	0.004
23	21.243	1030	134	0.003
24	22.245	2284	189	0.006
25	22.357	1049	190	0.003
26	22.735	1714	184	0.005
27	23.575	1670	216	0.005
28	23.678	2629	301	0.007
Total		35333503	2538770	100.000