

Sample Name :C-Peptide (3-33), human
 Cat No. :RP11116
 Lot No. :E4264520L
 Time Processed :8:36:58 AM
 Month-Day-Year Processed :12/26/20

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

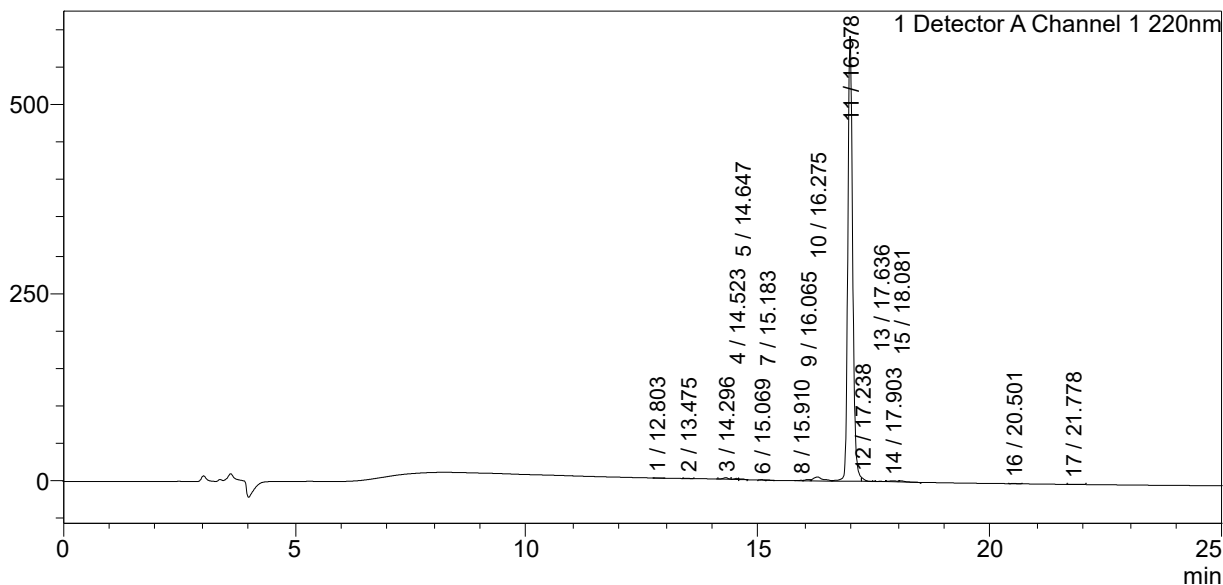

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.803	1184	182	0.026
2	13.475	1992	331	0.044
3	14.296	13943	2081	0.310
4	14.523	7105	1226	0.158
5	14.647	4674	907	0.104
6	15.069	2265	420	0.050
7	15.183	3033	544	0.067
8	15.910	3161	512	0.070
9	16.065	12363	1772	0.274
10	16.275	74418	5251	1.652
11	16.978	4326675	590812	96.052
12	17.238	18311	4802	0.406
13	17.636	2740	298	0.061
14	17.903	15284	1292	0.339
15	18.081	13290	1419	0.295

Peak#	Ret. Time	Area	Height	Area%
16	20.501	2647	421	0.059
17	21.778	1449	172	0.032
Total		4504532	612443	100.000