

Sample Name ::[Nle4, D-Phe7]- α -MSH, amide
 Cat. No. :RP10658
 Lot. No. :PE7941902
 Time Processed : 0:58:27
 Month-Day-Year Processed : 03/02/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

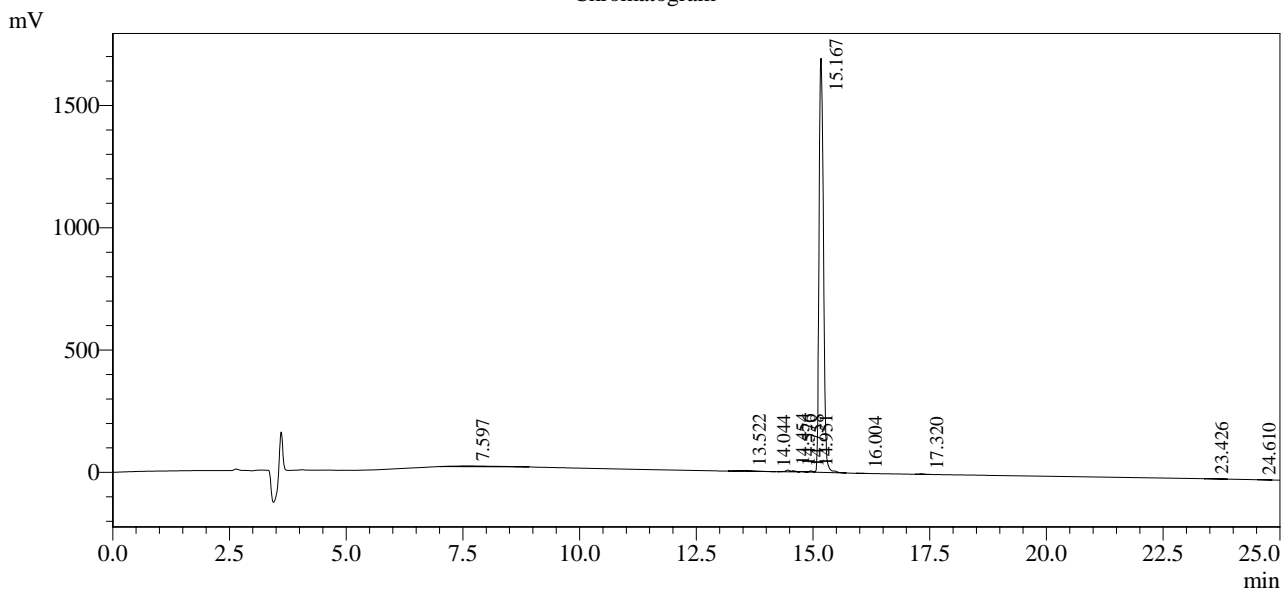

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	7.597	199978	2953	1.732
2	13.522	71651	2592	0.621
3	14.044	1286	206	0.011
4	14.454	42280	7233	0.366
5	14.576	23960	4520	0.208
6	14.758	10575	2117	0.092
7	14.951	25216	4712	0.218
8	15.167	11144749	1692928	96.523
9	16.004	3330	428	0.029
10	17.320	12641	2026	0.109
11	23.426	6224	312	0.054
12	24.610	4367	526	0.038
Total		11546257	1720551	100.000