

Sample Name : β -Amyloid (25-35)
 Cat No. :RP10008
 Lot No. :E8100821C
 Time Processed :7:21:53
 Month-Day-Year Processed :03/14/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

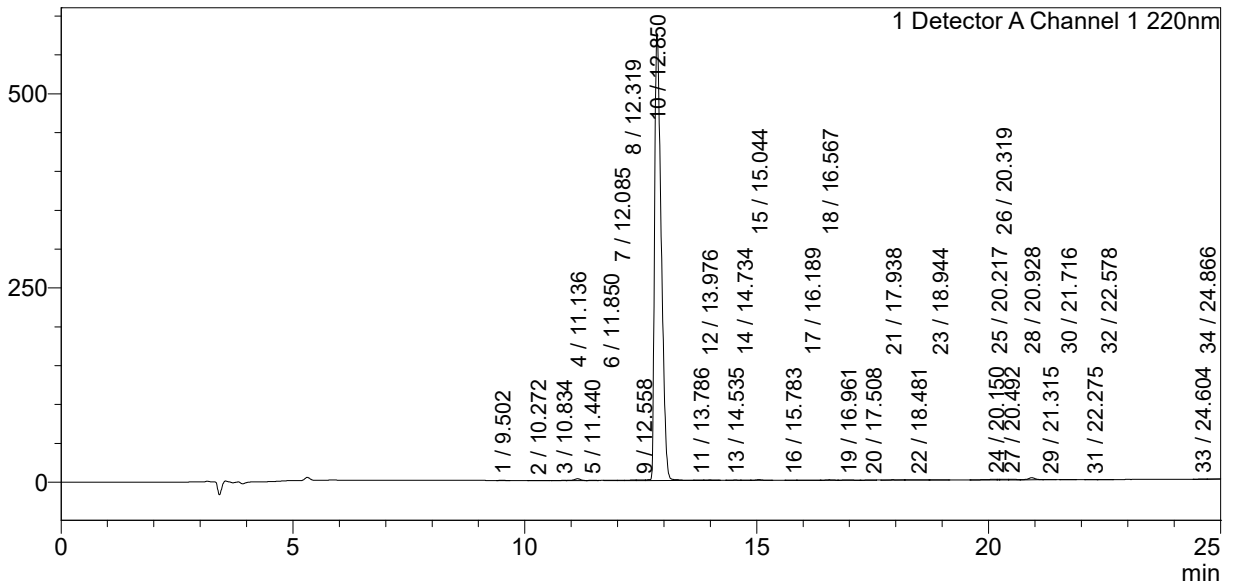

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.502	1215	173	0.021
2	10.272	1282	85	0.022
3	10.834	2000	179	0.034
4	11.136	21752	2250	0.369
5	11.440	2294	244	0.039
6	11.850	3771	325	0.064
7	12.085	1984	250	0.034
8	12.319	6090	526	0.103
9	12.558	8106	801	0.137
10	12.850	5736759	575275	97.268
11	13.786	1094	152	0.019
12	13.976	3154	270	0.053
13	14.535	3047	348	0.052
14	14.734	1711	173	0.029

Peak#	Ret. Time	Area	Height	Area%
15	15.044	7212	791	0.122
16	15.783	1220	98	0.021
17	16.189	3353	166	0.057
18	16.567	5613	566	0.095
19	16.961	2865	172	0.049
20	17.508	2230	181	0.038
21	17.938	7148	414	0.121
22	18.481	4680	201	0.079
23	18.944	1972	141	0.033
24	20.150	10480	629	0.178
25	20.217	2174	628	0.037
26	20.319	6902	625	0.117
27	20.492	7090	537	0.120
28	20.928	29083	2676	0.493
29	21.315	2574	187	0.044
30	21.716	2985	229	0.051
31	22.275	1032	80	0.017
32	22.578	1129	88	0.019
33	24.604	2217	233	0.038
34	24.866	1691	139	0.029
Total		5897910	589834	100.000