

Sample Name :HA Peptide  
 Cat No. :RP11735  
 Lot No. :E4734220K  
 Time Processed :1:00:33  
 Month-Day-Year Processed :11/12/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010141

<Chromatogram>

mV

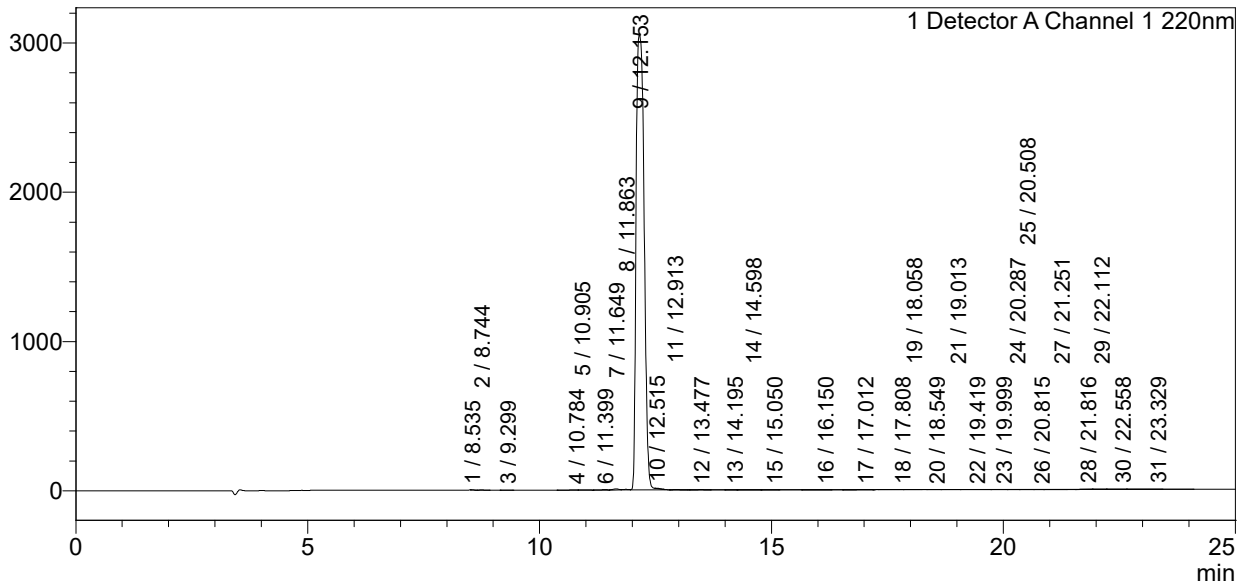

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.535	2002	576	0.005
2	8.744	7241	1087	0.020
3	9.299	1183	142	0.003
4	10.784	13122	1578	0.036
5	10.905	17047	1617	0.047
6	11.399	34068	3430	0.093
7	11.649	75528	8270	0.206
8	11.863	44435	4172	0.121
9	12.153	36340094	3058275	99.167
10	12.515	9779	1484	0.027
11	12.913	14776	1023	0.040
12	13.477	20995	2056	0.057
13	14.195	1399	134	0.004
14	14.598	9346	757	0.026

Peak#	Ret. Time	Area	Height	Area%
15	15.050	1360	148	0.004
16	16.150	2917	105	0.008
17	17.012	5150	208	0.014
18	17.808	3381	133	0.009
19	18.058	5615	508	0.015
20	18.549	2180	186	0.006
21	19.013	3733	190	0.010
22	19.419	8420	373	0.023
23	19.999	3294	189	0.009
24	20.287	2142	164	0.006
25	20.508	1766	143	0.005
26	20.815	1012	116	0.003
27	21.251	2705	171	0.007
28	21.816	3706	283	0.010
29	22.112	3417	256	0.009
30	22.558	2330	115	0.006
31	23.329	1360	87	0.004
Total		36645503	3087977	100.000