


# Mass Spectrum

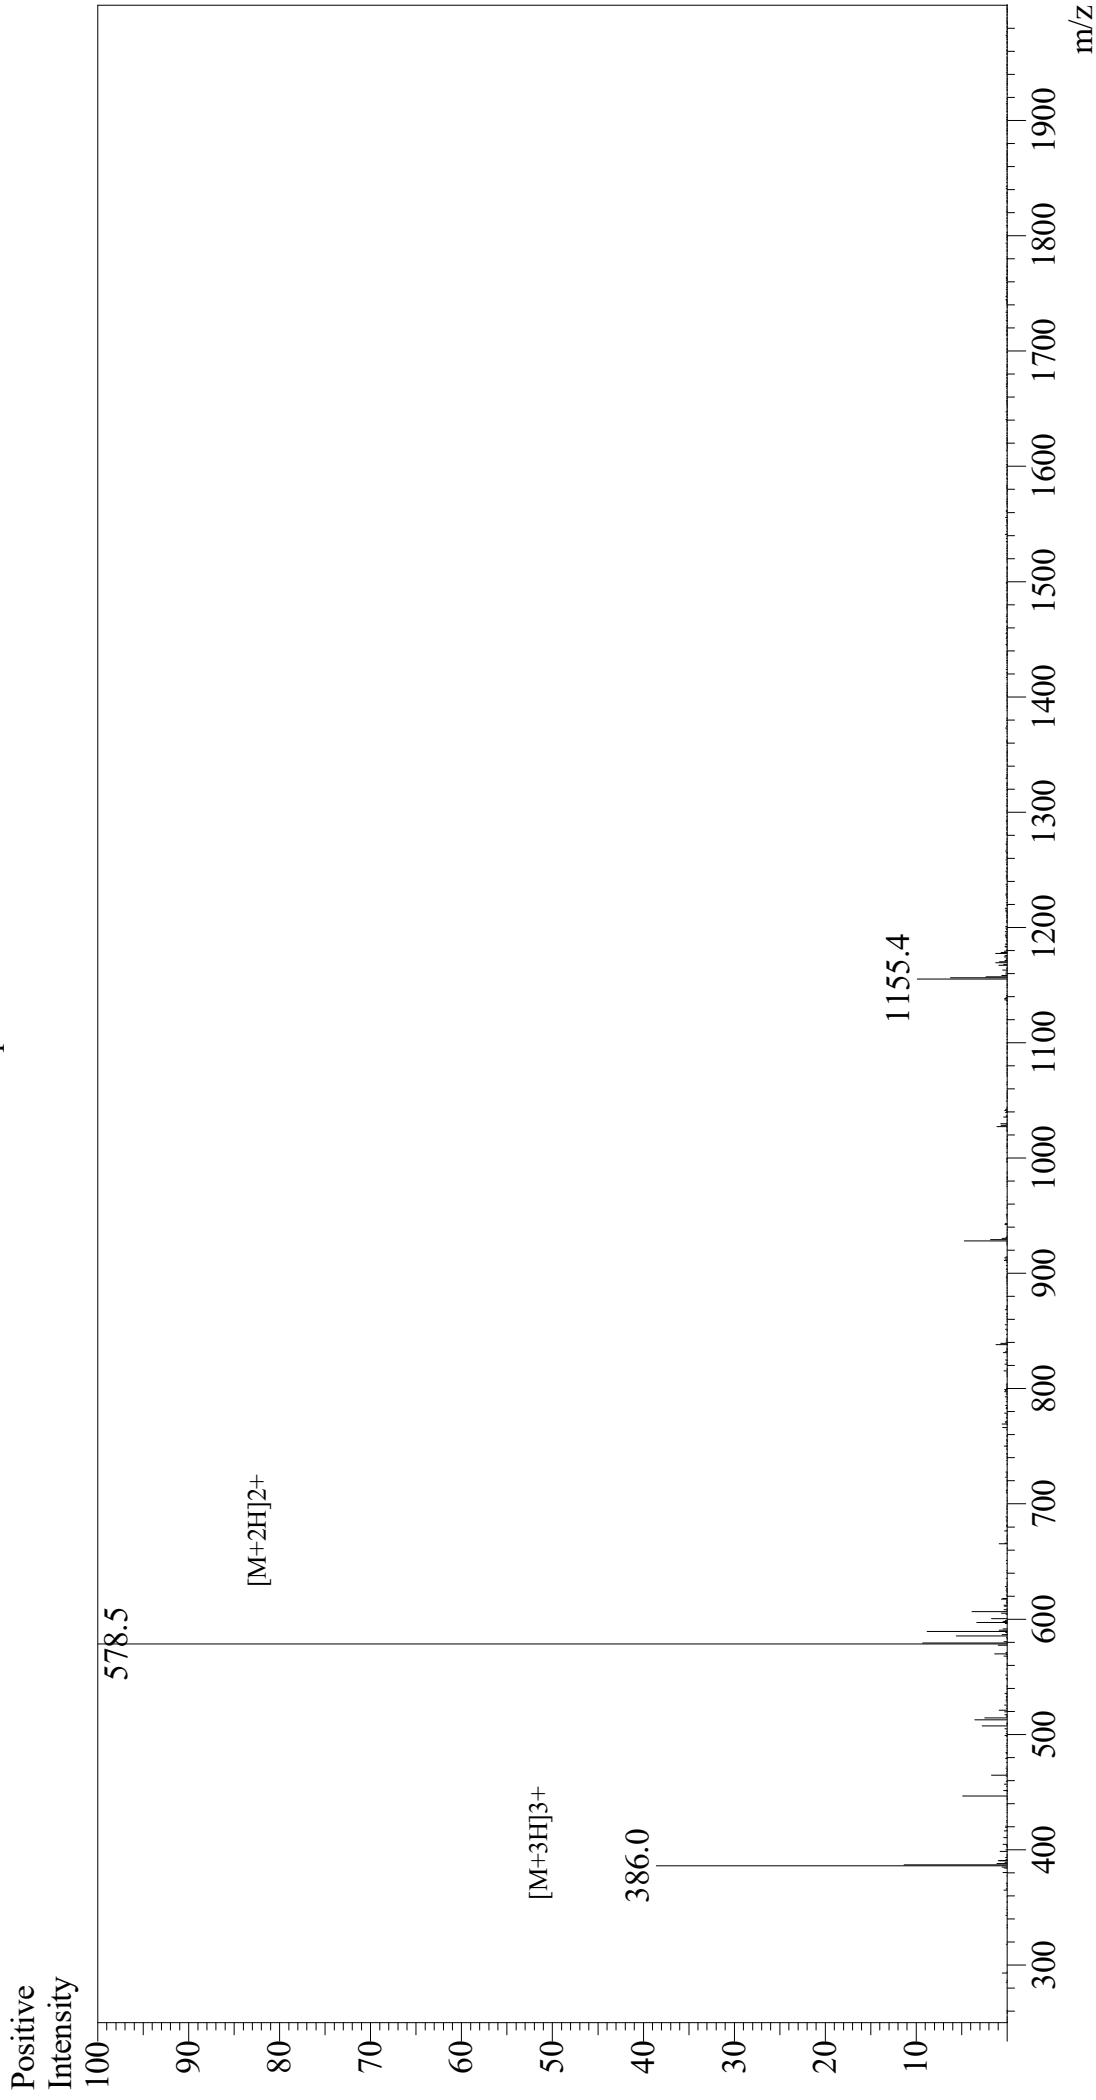

## Sample Information

Month-Day/Processed : 12/22/20  
Time Processed : 10:48:54 PM  
Injection Volume : 0.4  
Sample Name : hgp100(25-33)  
Cat No. : RP20344  
Lot No. : E7983820L  
Theoretical MW : 1155.30  
Observed MW : 1155.0

Interface : ESI  
Nebulizing Gas Flow : 1.5L/min  
CDL Temp : 250  
Block Temp : 200

Equipment : GK11010007  
Interface Bias : +3.5 kV  
Drying Gas Flow : 5 L/min  
T.Flow : 0.2 ml/min  
B.conc : 50%H2O/50%MeOH