

Sample Name : Neuropeptide Y, human
 Cat. No. : RP10492
 Lot. No. : E1707319J
 Time Processed :7:34:40
 Month-Day-Year Processed :10/24/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

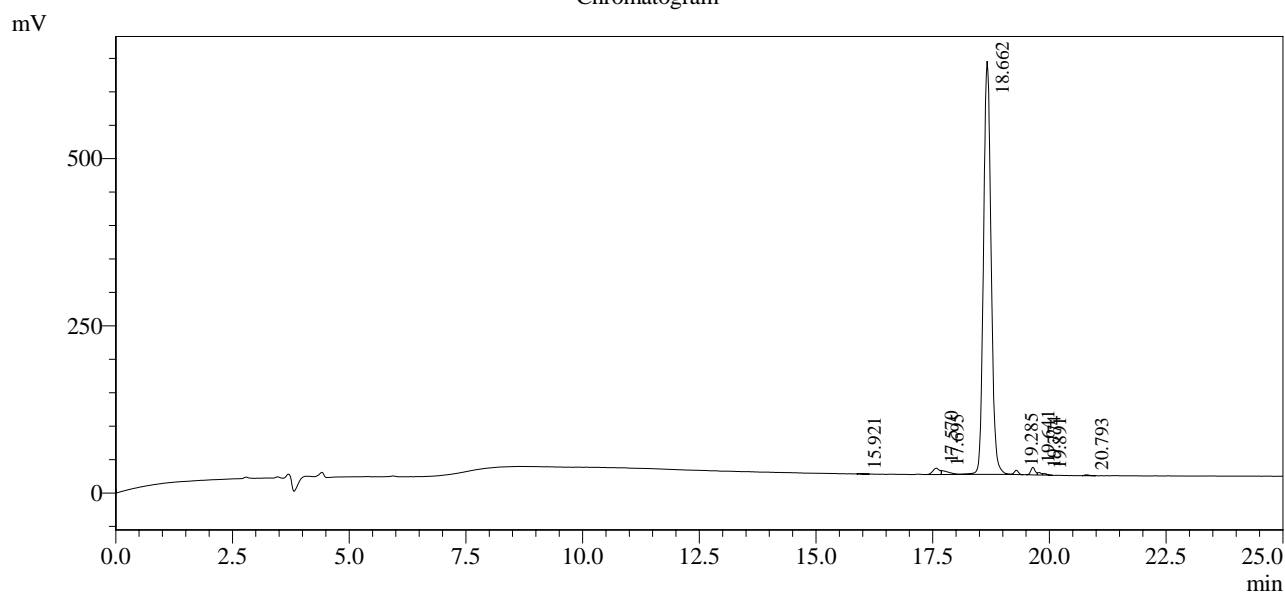

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.921	1394	298	0.019
2	17.570	95801	9458	1.312
3	17.695	63262	5586	0.866
4	18.662	6989836	617802	95.727
5	19.285	37597	6297	0.515
6	19.641	72396	11130	0.991
7	19.774	18965	3626	0.260
8	19.891	12691	2208	0.174
9	20.793	9882	1314	0.135
Total		7301824	657719	100.000