

Sample Name : CGRP (8-37), rat
 Cat. No. : RP11090
 Lot. No. : PE1741807

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

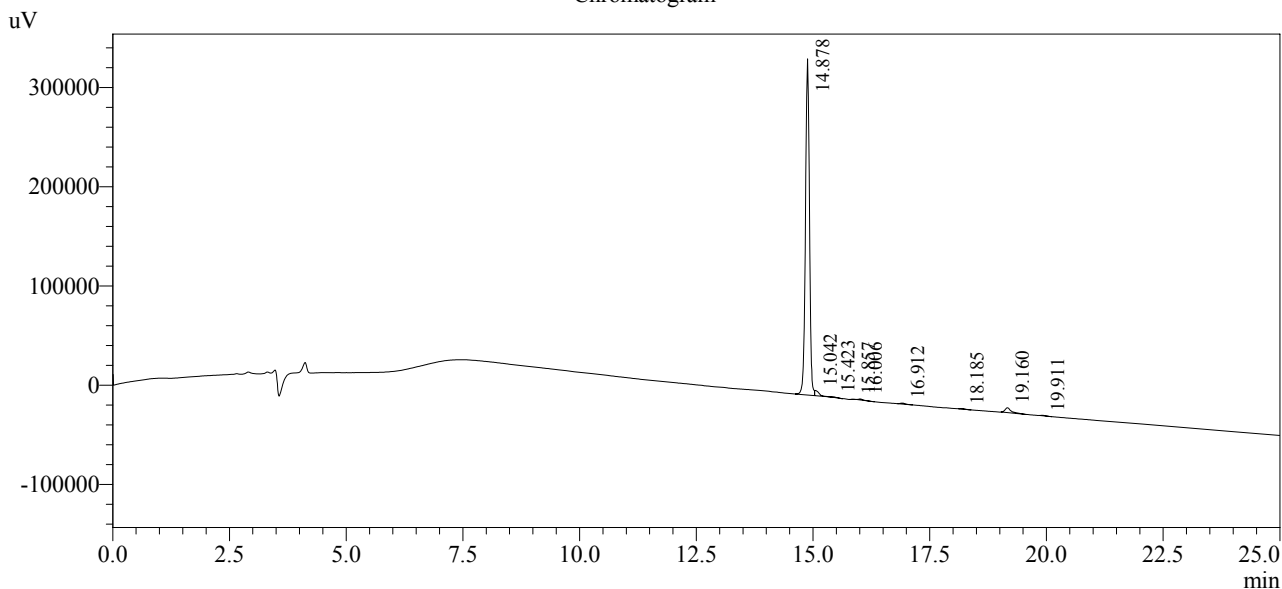

1 Det. A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.878	2008867	338871	95.123
2	15.042	32798	5289	1.553
3	15.423	4174	456	0.198
4	15.857	1332	317	0.063
5	16.006	6945	1015	0.329
6	16.912	6440	950	0.305
7	18.185	3513	521	0.166
8	19.160	44924	4868	2.127
9	19.911	2868	406	0.136
Total		2111862	352692	100.000